

# START

9613428.0856

LK5106-LAS  
122  
2

0043954

Lockheed Analytical Services

Log-in No.: L5106  
Quotation No.: Q400000-B  
SAF: B95-068  
Document File No.: 0811596  
WHC Document File No.: 257  
SDG No.: LK5106  
Page 2



## CASE NARRATIVE INORGANIC NON METALS ANALYSES

The routine calibration and quality control analyses performed for this batch include as applicable: instrument tune (ICP/MS only), initial and continuing calibration verification, initial and continuing calibration blanks, method blank(s), laboratory control sample(s), ICP interference check samples (ICP only), serial dilutions, analytical (post-digestion) spike samples, matrix spike (predigestion) sample(s), duplicate sample(s).

### Preparation and Analysis Requirements

- One water sample was received for LK5106 and analyzed in batch 811 bh for selected analytes as requested on the chain of custody. Quality control analysis was performed on the following sample:

Client ID	LAL #		Method
BOGFD7	L5106-3	MS, DUP	300.0 Chloride, Fluoride, Nitrate-Nitrogen, Nitrite-Nitrogen, Orthophosphate, Sulfate
	L5106-6	MS, DUP	350.1 Ammonia
	L5106-4	MS, DUP	353.2 Nitrate-Nitrite-Nitrogen
	L5106-5	MS, DUP	9030 Sulfide

### Holding Time Requirements

- All samples were analyzed within the method-specific holding time with the exception of Method 300.0 Nitrate-Nitrogen, Nitrite-Nitrogen and Orthophosphate which were received outside of holding time. The associated samples are flagged with an "H".

### Method Blanks

- The concentration levels of all the requested analytes in the method blank were below the reporting detection limits.

### Internal Quality Control

- All Internal Quality Control were within acceptance limits.

Kay McCann  
Prepared By

September 12, 1995  
Date

0006

**Lockheed Analytical Services**

Log-in No.: L5106  
Quotation No.: Q400000-B  
SAF: B95-068  
Document File No.: 0811596  
WHC Document File No.: 257  
SDG No.: LK5106  
Page 3

## **CASE NARRATIVE INORGANIC METALS ANALYSES**

The routine calibration and quality control analyses performed for this batch include as applicable: instrument tune (ICP/MS only), initial and continuing calibration verification, initial and continuing calibration blanks, method blank(s), laboratory control sample(s), ICP interference check samples (ICP only), serial dilutions, analytical (post-digestion) spike samples, matrix spike (predigestion) sample(s), duplicate sample(s).

### **Preparation and Analysis Requirements**

- One water sample for total metals analysis. The sample was prepared as LAS Batch 811BHT and analyzed for selected analytes as requested on the chain of custody. Sample BOGFD7 (L5106-2) was used for matrix spike and duplicate and serial dilution. All data flags due to the performance of the above-mentioned QC are also associated with every sample digested with this batch.

### **Holding Time Requirements**

- All samples were analyzed within the method-specific holding times.

### **Internal Quality Control**

- All internal quality control were within acceptance limits with the following exceptions:  
  
For lead, the LCSW (121.1%) recovered slightly above the acceptance criteria (80-120%). No lead was detected in the sample, therefore the positive bias observed does not affect the result. No corrective action was taken.

### **Sample Results**

- The following qualifiers are reported on the basis of the techniques employed to perform the analyses:

"P" ICP-AES

Nalini Prabhakar

09/08/95

Prepared By

Date

*Lockheed Analytical Services*

Log-in No.: L5106  
Quotation No.: Q400000-B  
SAF: B95-068  
Document File No.: 0811596  
WHC Document File No.: 257  
SDG No.: LK5106  
Page 4

## CASE NARRATIVE INORGANIC METALS ANALYSES

The routine calibration and quality control analyses performed for this batch include as applicable: instrument tune (ICP/MS only), initial and continuing calibration verification, initial and continuing calibration blanks, method blank(s), laboratory control sample(s), ICP interference check samples (ICP only), serial dilutions, analytical (post-digestion) spike samples, matrix spike (predigestion) sample(s), duplicate sample(s).

### Preparation and Analysis Requirements

- One filtered water sample was analyzed for dissolved metals analysis. As the measured turbidity of the sample was less than 1 NTU, it was batched as LAS batch 811BHD for dissolved metals analysis. Sample BOGFD8 (L5106-13) was used for matrix spike, duplicate and serial dilution analyses. All data flags due to the performance of the above-mentioned QC sample are also associated with every sample analyzed with this batch.

### Holding Time Requirements

- All samples were analyzed within the method-specific holding times.

### Method Blanks

- The level of analytes in the method blanks were less than the reporting detection limits.

### Internal Quality Control

All internal quality control were within acceptance limits with the following exceptions:

- In the analysis of calcium, the percent difference of serial dilution slightly exceeded 10% the control limit. This may be due to physical interferences. Calcium results for the associated sample is flagged with an "E".

### Sample Results

- The following qualifiers are reported on the basis of the techniques employed to perform the analyses:  
"P" ICP-AES

Nalini Prabhakar  
Prepared By

09/08/95  
Date

0008

**Lockheed Analytical Services**

Log-in No.: L5106  
Quotation No.: Q400000-B  
SAF: B95-068  
Document File No.: 0811596  
WHC Document File No.: 257  
SDG No.: LK5106  
Page 5

## **CASE NARRATIVE RADIOCHEMICAL ANALYSES**

The routine calibration and quality control (QC) analyses performed for this batch include as applicable: instrument calibration, initial and continuing calibration verification, quench monitoring standards, instrument background analysis, method blanks, yield tracer, laboratory control samples, matrix spike samples, duplicate samples.

**NOTE:** Chemical recoveries and minimum detectable activities can be found on the preparation sheets and calculation sheets on the attached raw data for each method.

### **Holding Time Requirements**

All holding times were met.

### **Analytical Method Gross Alpha/Beta**

The gross alpha/beta analysis was performed using standard operating procedure (SOP), LAL-91-SOP-0060. The samples were analyzed in workgroup 26272. No problems were encountered during analysis and all QC criteria were met. No re-analyses were performed.

### **Analytical Method Strontium-90**

The strontium-90 analysis was performed using SOP, LAL-91-SOP-0196. The samples were analyzed in workgroup 26273. No problems were encountered during the analysis and all QC criteria were met with the following exceptions: The relative error recovery and relative percent difference were slightly out of QC criteria. Data quality is not adversely affected. No re-analyses were performed.

### **Analytical Method Tritium**

The tritium analysis was performed using SOP, LAL-91-SOP-0066. The samples were analyzed in workgroup 26274. No problems were encountered during analysis and all QC criteria were met. No re-analyses were performed.

Andrea Tippett  
Prepared By

August 26, 1995  
Date

0009

9613428.0840

LOCKHEED ANALYTICAL SERVICES  
 LOGIN CHAIN OF CUSTODY REPORT (1n01)  
 Aug 11 1995, 04:16 pm

Login Number: L5106  
 Account: 596 Bechtel Hanford, Inc. \* Richland, WA  
 Project: BECHTEL-HANFORD Bechtel Hanford Project

Laboratory Sample Number	Client Sample Number	Collect Date	Receive Date	Due PR Date
L5106-1 temp 2; B95-068 Location: 157 Water 1 S SCREENING	BOGFD7	09-AUG-95	11-AUG-95	25-SEP-95
			Hold:05-FEB-96	
L5106-2 temp 2; B95-068 Location: 157 Water 1 S 6010 ICP METALS	BOGFD7	09-AUG-95	11-AUG-95	25-SEP-95
			Hold:05-FEB-96	
L5106-3 temp 2; B95-068 Location: 157 Water 1 S 300.0 CHLORIDE Water 1 S 300.0 FLUORIDE Water 1 S 300.0 NITRATE Water 1 S 300.0 NITRITE Water 1 S 300.0 PHOSPHATE Water 1 S 300.0 SULFATE	BOGFD7	09-AUG-95	11-AUG-95	25-SEP-95
			Hold:06-SEP-95 Hold:06-SEP-95 Hold:11-AUG-95 Hold:11-AUG-95 Hold:11-AUG-95 Hold:06-SEP-95	
L5106-4 temp 2; B95-068 Location: 157 Water 1 S 353.2 NITRATE	BOGFD7	09-AUG-95	11-AUG-95	25-SEP-95
			Hold:06-SEP-95	
L5106-5 temp 2; B95-068 Location: 157 Water 1 S 9030 SULFIDE	BOGFD7	09-AUG-95	11-AUG-95	25-SEP-95
			Hold:16-AUG-95	
L5106-6 temp 2; B95-068 Location: 157 Water 1 S 350.1 NH3/N	BOGFD7	09-AUG-95	11-AUG-95	25-SEP-95
			Hold:06-SEP-95	
L5106-7 temp 2; B95-068 Location: 157 Water 1 S GR ALP/BETA LAL-0060 Water 1 S SR-90 LAL-0196	BOGFD7	09-AUG-95	11-AUG-95	25-SEP-95
			Hold:05-FEB-96 Hold:05-FEB-96	
L5106-8 temp 2; B95-068 Location: 157	BOGFD7	09-AUG-95	11-AUG-95	25-SEP-95

9615428.0041

LOCKHEED ANALYTICAL SERVICES  
 LOGIN CHAIN OF CUSTODY REPORT (ln01)  
 Aug 11 1995, 04:16 pm

Login Number: L5106  
 Account: 596 Bechtel Hanford, Inc. \* Richland, WA  
 Project: BECHTEL-HANFORD Bechtel Hanford Project

Laboratory Sample Number	Client Sample Number	Collect Date	Receive Date	Due PR Date
L5106-9 temp 2; B95-068 Location: 157	BOGFD7	09-AUG-95	11-AUG-95	25-SEP-95
L5106-10 temp 2; B95-068 Location: 157	BOGFD7	09-AUG-95	11-AUG-95	25-SEP-95
L5106-11 temp 2; B95-068 Location: 157	BOGFD7	09-AUG-95	11-AUG-95	25-SEP-95
L5106-12 temp 2; B95-068 Location: 157 Water 1 S TRITIUM(H3) LAL-0066 Hold:05-FEB-96	BOGFD7	09-AUG-95	11-AUG-95	25-SEP-95
L5106-13 temp 2; B95-068 Location: 157 Filt H2O 15 S 6010 ICP METALS Hold:05-FEB-96	BOGFD8	09-AUG-95	11-AUG-95	25-SEP-95
L5106-14 B95-068 Location: Water 1 S EDD - DISK DEL. Water 1 S INORG TYPE 4A RPT Water 1 S RAD RPT TYPE 4F	REPORT TYPE	11-AUG-95	11-AUG-95	25-SEP-95

Signature: *[Handwritten Signature]*

Date: 8-11-95

0014

081159C

Bechtel Hanford, Inc.

# L5106 CHAIN OF CUSTODY/SAMPLE ANALYSIS REQUEST

Data Turnaround  
 Priority  
 Normal

Collector <i>K.D Lee</i>	Company Contact R. E. Peterson	Telephone (509) 372-9638
Project Designation 100-HR-3 Groundwater Sampling, Round 9, Phase 2	Sampling Location 100 D	SAF No. B95-068
Ice Chest No. <i>Patton</i>	Field Logbook No. <i>E.F.L.-1018</i>	Method of Shipment Federal Express
Shipped To Lockheed	Offsite Property No. NA <i>8-145</i> <i>W95-0-0204-46</i>	Bill of Lading/Air Bill No. <i>2904637303</i>

Possible Sample Hazards/Remarks	Preservation	HNO <sub>3</sub>	Cool 4°C	H <sub>2</sub> SO <sub>4</sub>	*1	H <sub>2</sub> SO <sub>4</sub>	HNO <sub>3</sub>	Cool 4°C	Cool 4°C		HNO <sub>3</sub>
	Type of Container	G	G	P/G	P	P/G	P/G	G	P/G		G
	No. of Container(s)	1	1	1	1	1	5	1	1		1
Special Handling and/or Storage Maintain samples between 2°C and 6°C.	Volume	500mL	500mL	500mL	1L	1L	1L	500mL	20mL		500mL

SAMPLE ANALYSIS				ICP Metals (Unfiltered)	Anions (IC) - F, Cl, SO <sub>4</sub> , NO <sub>2</sub> , NO <sub>3</sub> , PO <sub>4</sub>	NO <sub>2</sub> - NO <sub>3</sub>	Sulfide	Ammonia	Gross Alpha, Gross Beta, Sr-90	Tritium	Activity Scan	ICP Metals (Filtered)
-----------------	--	--	--	-------------------------	--	-----------------------------------	---------	---------	--------------------------------	---------	---------------	-----------------------

Sample No.	Matrix*	Date Sampled	Time Sampled	ICP Metals (Unfiltered)	Anions (IC)	NO <sub>2</sub> - NO <sub>3</sub>	Sulfide	Ammonia	Gross Alpha, Gross Beta, Sr-90	Tritium	Activity Scan	ICP Metals (Filtered)
BOGFD7	W	8/9/95	1138	X	X	X	X	X	X	X	X	
BOGFD8	W	8/9/95	1135									X

CHAIN OF POSSESSION		Sign/Print Names		SPECIAL INSTRUCTIONS *1 ZnAc + NaOH				Matrix*	
Relinquished By <i>K.D Lee</i>	Date/Time <i>8/10/95 0730</i>	Received By <i>BRE</i>	Date/Time <i>0730</i>	Sample analysis for phosphate, nitrate, and nitrite by EPA 300.0; end turbidity by EPA 180.1 is being requested for information only. The ERC Contractor acknowledges that the 48-hour holding time will not be met.  The Activity Scan is for all samples listed on this chain of custody.				<ul style="list-style-type: none"> <li>S - Soil</li> <li>SE - Sediment</li> <li>SO - Solid</li> <li>SL - Sludge</li> <li>W - Water</li> <li>O - Oil</li> <li>A - Air</li> <li>DS - Drum Solids</li> <li>DL - Drum Liquids</li> <li>T - Tissue</li> <li>WI - Wipe</li> <li>L - Liquid</li> <li>V - Vegetation</li> <li>X - Other</li> </ul>	
Relinquished By <i>K.D Lee</i>	Date/Time <i>0830</i>	Received By <i>B.W.H.H.</i>	Date/Time <i>8-10-95</i>						
Relinquished By <i>K.D Lee</i>	Date/Time <i>8-10-95</i>	Received By	Date/Time						
Relinquished By <i>K.D Lee</i>	Date/Time	Received By	Date/Time						

LABORATORY SECTION	Received By <i>K.D Lee</i>	Title <i>Sample Custodian</i>	Date/Time <i>8-11-95 0730</i>
FINAL SAMPLE DISPOSITION	Disposal Method	Disposed By	Date/Time

76181594

2904637303

### SAMPLE CHECK-IN LIST

Date/Time Received: 8-11-95/0920 SDG#: N/A

Work Order Number: N/A SAF #: 895-068

Shipping Container ID: Packer Chain of Custody #: N/A

- 1. Custody Seals on shipping container intact? Yes  No
- 2. Custody Seals dated and signed? Yes  No
- 3. Sample temperature 2°C
- 4. Vermiculite/packing materials is Wet  Dry
- 5. Each sample is in a plastic bag? Yes  No
- 6. Sample holding times exceeded? Yes  No

7. Samples have:  
 tape  hazard labels  
 custody seals  appropriate sample labels

8. Samples are:  
 in good condition  leaking  
 broken  have air bubbles

9. Is the information on the COC and Sample bottles in agreement?

Yes  No

Notes: \_\_\_\_\_  
\_\_\_\_\_  
\_\_\_\_\_

Sample Custodian/Laboratory: Johny G Date: 8-11-95

Telephoned To: Kathleen Hall On 8-11-95 By Anthony Miller

9613428.0844

## LOCKHEED ANALYTICAL SERVICES

## Sample Results

Client Sample ID: B0GFD7	Date Collected: 09-AUG-95
Matrix: Water	Date Received: 11-AUG-95
Percent Solids: N/A	

Constituent	Units	Method	Result	Project Reporting Limit	Data Qualifier(s)	Date Analyzed	LAS Batch ID	LAS Sample ID
Chloride	mg/L	300.0	27.	0.020		14-AUG-95	26209	L5106-3
Fluoride	mg/L	300.0	< 0.001	0.10	U	05-SEP-95	26210	L5106-3
Nitrate-N	mg/L	300.0	35.	0.020	H	14-AUG-95	26211	L5106-3
Nitrite-N	mg/L	300.0	< 0.002	0.010	HU	14-AUG-95	26212	L5106-3
Ortho Phosphate	mg/L	300.0	< 0.020	0.10	HU	14-AUG-95	26213	L5106-3
Sulfate	mg/L	300.0	130	0.10		14-AUG-95	26214	L5106-3
Ammonia Nitrogen	mg/L	350.1	0.46	0.050		16-AUG-95	26215	L5106-6
Nitrate-Nitrite-Nitrogen	mg/L	353.2	35.	0.50	D(1:10)	18-AUG-95	26217	L5106-4
Sulfide	mg/L	9030	< 1.0	3.0	U	15-AUG-95	26249	L5106-5

0023

9613428.0845

SW - 846

1  
INORGANIC ANALYSES DATA SHEET

CLIENT ID NO.

BOGFD7

Lab Name: L.A.S \_\_\_\_\_ Contract: HANFORD \_\_\_\_\_

Lab Code: LOCK \_\_\_\_\_ Case No.: B95-06 SAS No.: \_\_\_\_\_ SDG No.: L5106W

Matrix (soil/water): WATER Lab Sample ID: L5106-2 \_\_\_\_\_

Level (low/med): LOW \_\_\_\_\_ Date Received: 08/11/95

% Solids: \_\_\_\_\_ 0

Concentration Units (ug/L or mg/kg dry weight): UG/L \_\_\_\_\_

CAS No.	Analyte	Concentration	C	Q	M
7429-90-5	Aluminum	29.0	U		P
7440-36-0	Antimony	58.0	U		P
7440-38-2	Arsenic	98.0	U		P
7440-39-3	Barium	146	B		P
7440-41-7	Beryllium	1.0	U		P
7440-43-9	Cadmium	5.0	U		P
7440-70-2	Calcium	122000			P
7440-47-3	Chromium	170			P
7440-48-4	Cobalt	6.0	U		P
7440-50-8	Copper	3.0	U		P
7439-89-6	Iron	105			P
7439-92-1	Lead	56.0	U		P
7439-95-4	Magnesium	12400			P
7439-96-5	Manganese	2.0	U		P
7440-02-0	Nickel	15.0	U		P
7440-09-7	Potassium	7850			P
7782-49-2	Selenium	87.0	U		P
7440-22-4	Silver	4.0	U		P
7440-23-5	Sodium	8220			P
7440-28-0	Thallium	50.0	U		P
7440-62-2	Vanadium	4.0	U		P
7440-66-6	Zinc	7.8	B		P

Color Before: COLORLESS Clarity Before: CLEAR \_\_\_\_\_ Texture: \_\_\_\_\_

Color After: COLORLESS Clarity After: CLEAR \_\_\_\_\_ Artifacts: \_\_\_\_\_

Comments:

\_\_\_\_\_  
\_\_\_\_\_  
\_\_\_\_\_

9613428.0846

SW - 846

1  
INORGANIC ANALYSES DATA SHEET

CLIENT ID NO.

BOGFD8

Lab Name: L.A.S \_\_\_\_\_ Contract: HANFORD \_\_\_\_\_

Lab Code: LOCK \_\_\_\_\_ Case No.: B95-06 SAS No.: \_\_\_\_\_ SDG No.: L5106F

Matrix (soil/water): WATER Lab Sample ID: L5106-13 \_\_\_\_\_

Level (low/med): LOW \_\_\_\_\_ Date Received: 08/11/95

% Solids: \_\_\_\_\_ 0

Concentration Units (ug/L or mg/kg dry weight): UG/L \_\_\_\_\_

CAS No.	Analyte	Concentration	C	Q	M
7429-90-5	Aluminum	30.3	B		P
7440-36-0	Antimony	58.0	U		P
7440-38-2	Arsenic	98.0	U		P
7440-39-3	Barium	141	B		P
7440-41-7	Beryllium	1.0	U		P
7440-43-9	Cadmium	5.0	U		P
7440-70-2	Calcium	124000		E	P
7440-47-3	Chromium	158			P
7440-48-4	Cobalt	6.0	U		P
7440-50-8	Copper	3.0	U		P
7439-89-6	Iron	12.0	U		P
7439-92-1	Lead	65.0	B		P
7439-95-4	Magnesium	12200			P
7439-96-5	Manganese	2.0	U		P
7440-02-0	Nickel	15.0	U		P
7440-09-7	Potassium	7580			P
7782-49-2	Selenium	87.0	U		P
7440-22-4	Silver	4.0	U		P
7440-23-5	Sodium	7800			P
7440-28-0	Thallium	109	B		P
7440-62-2	Vanadium	5.3	B		P
7440-66-6	Zinc	8.7	B		P

Color Before: \_\_\_\_\_ Clarity Before: \_\_\_\_\_ Texture: \_\_\_\_\_

Color After: \_\_\_\_\_ Clarity After: \_\_\_\_\_ Artifacts: \_\_\_\_\_

Comments:

\_\_\_\_\_  
\_\_\_\_\_  
\_\_\_\_\_

9613428.0847

LOCKHEED ANALYTICAL SERVICES

RAD DATA REPORT (ra01)

Bechtel Hanford, Inc. \* Richland, WA

Bechtel Hanford Project (Project BECHTEL-HANFORD)

Client Sample ID: BOGFD7

LAL Sample ID: L5106-7

Date Collected: 09-AUG-95

Date Received: 11-AUG-95

Matrix: Water

Login Number: L5106

Constituent	Analyzed	Batch	Activity	Error	MDA	DataQual	Units
Gross Alpha	23-AUG-95	GR ALP/BETA LAL-0060_26272	3.7	2.6	3.5	C	pCi/L
Gross Beta	23-AUG-95	GR ALP/BETA LAL-0060_26272	11.3	2.7	3.4		pCi/L
Total radio-strontium	18-AUG-95	SR-90 LAL-0196_26273	4.37	0.63	0.72		pCi/L

9613428.0848

LOCKHEED ANALYTICAL SERVICES

RAD DATA REPORT (ra01)

Bechtel Hanford, Inc. \* Richland, WA

Bechtel Hanford Project (Project BECHTEL-HANFORD)

Client Sample ID: BOGFD7

LAL Sample ID: L5106-12

Date Collected: 09-AUG-95

Date Received: 11-AUG-95

Matrix: Water

Login Number: L5106

Constituent	Analyzed	Batch	Activity	Error	MDA	DataQual	Units
H-3	24-AUG-95	TRITIUM(H3) LAL-0066_26274	3680	480	270		pCi/L

9613428.0849



Los Alamos Technical Associates, Inc.

8633 Gage Blvd. / Kennewick, WA 99336 / Telephone (509) 783-4369 / FAX (509) 783-9661

November 10, 1995  
LATA95-217



Ms. Joan Kessner  
Bechtel  
1022 Lee Boulevard  
Richland, WA 99352

Subject: VB404.05, SDG LK5106-LAS

Dear Ms. Kessner:

Attached is the data validation report for analytical results for 100-HR-3 Groundwater Round 9 - Phase II, (SDG LK5106-LAS). The package was received by Los Alamos Technical Associates on October 12, 1995. This data package was initially placed on hold October 17, 1995 to request missing information deemed necessary to the validation effort. The final information request was closed on October 31, 1995 placing the package back in active status.

If you have any questions, please feel free to contact me.

Sincerely,

*Brent Mowbray for*

Marsha C. Webb  
Deputy Project Manager

Attachment

cc: Jeanette Duncan, CH2M Hill  
Don Smith, LATA  
VB404.05  
MCW/lb

In

**DATA VALIDATION REPORT**  
**for**  
**100-HR-3 GROUNDWATER ROUND 9**  
**PHASE II**  
**Metals Analysis**  
**SDG LK5106-LAS**  
**LATA VB404.05**

Bechtel Hanford Inc.  
P.O. Box 969  
Richland, Washington

November 10, 1995

## Table of Contents

Data Validation Narrative .....	000002
INTRODUCTION .....	000002
ANALYSES REQUESTED .....	000002
DATA QUALITY OBJECTIVES .....	000002
REFERENCES .....	000004
GLOSSARY OF VALIDATION APPLIED QUALIFIERS (CHEMISTRY) .....	000005
GLOSSARY OF LABORATORY APPLIED QUALIFIERS .....	000006
Qualification Summary Table .....	000007
Data Summary Table .....	000009
Sample Results .....	000011
Checklist .....	000014
Laboratory Case Narrative .....	000033
Chain-of-Custody Information .....	000036
END OF PACKAGE .....	000038

100-HR-3 GROUNDWATER ROUND 9 PHASE II  
Data Validation Narrative

## INTRODUCTION

All samples in Sample Delivery Group (SDG) LK5106-LAS (VB404.05) were validated at level D as defined in the Data Validation Procedures for Chemical Analysis (WHC-SD-EN-SPP-002, Rev. 2).

The analyses were performed by Lockheed Analytical Services.

## ANALYSES REQUESTED

See Table 1.

## DATA QUALITY OBJECTIVES

- Precision:** Goals for precision were met with the exception of those items discussed in the **'Qualification Summary Table'**.
- Accuracy:** Goals for accuracy were met with the exception of those items discussed in the **'Qualification Summary Table'**.
- Sample Result Verification:** All sample results were supported in the raw data.
- Detection Limits:** Detection limit goals were met for all sample results as specified in the *RCRA Facility Investigation/Corrective Measures Study Work Plan for the 100-HR-3 Operable Unit*, DOE/RL-88-36, Rev. 0, with the exception of arsenic, lead, selenium and thallium.
- Completeness:** The data package was 100% complete for all requested analyses.

## MAJOR DEFICIENCIES

No major deficiencies were identified during data validation which required qualification of data as unusable.

## MINOR DEFICIENCIES

Minor deficiencies were identified during validation which required qualification of data as estimated. See the **'Qualification Summary Table'**.

9613428.0853

**Table 1**  
**Chain-of-Custody**  
**Analysis Request**

LATA ID #: VB404.05

SDG: LK5106-LAS

Sample Information					Analyses Requested	
SAMPLE NO.	DATE COLLECTED	MATRIX	SAF	FIELD QC INFO	1	2
B0GFD7	9-Aug-95	WATER	B95-068	Split of B0GFB1	X	
B0GFD8	9-Aug-95	WATER	B95-068	Split of B0GFB2		X

**Method References:**

<u>Analysis</u>	<u>Method</u>
1. ICP Metals (Unfiltered)	6010
2. ICP Metals (Filtered)	6010

**REFERENCES**

WHC 1993, *Data Validation Procedures for Chemical Analyses*, WHC-SD-EN-SPP-002, Rev. 2, Westinghouse Hanford Company, Richland, Washington.

DOE 1992, *RCRA Facility Investigation/Corrective Measures Study Work Plan for the 100-HR-3 Operable Unit*, DOE/RL-88-36, Rev. 0, Department of Energy-Hanford, Richland, Washington.

**GLOSSARY OF VALIDATION APPLIED QUALIFIERS (CHEMISTRY)**

Qualifiers which may be applied by data validators in compliance with the procedures herein are as follows.

- U- Indicates the compound or analyte was analyzed for and not detected in the sample. The value reported is the sample quantitation limit corrected for sample dilution and moisture content by the laboratory.
- UJ- Indicates the compound or analyte was analyzed for and not detected in the sample. Due to a QC deficiency identified during data validation, the associated quantitation limit is an estimate.
- J- Indicates the compound or analyte was analyzed for and detected. The associated concentration is an estimate, but the data are usable for decision making purposes.
- BJ- Applied to inorganic analyses only. Indicates the analyte concentration was greater than the IDL but less than the CRDL and is considered an estimated value.
- R- Indicates the compound or analyte was analyzed for, detected, and due to an identified QC deficiency the data are unusable.
- UR- Indicates the compound or analyte was analyzed for and not detected in the sample. Additionally, the data are unusable due to an identified QC deficiency.

**GLOSSARY OF LABORATORY APPLIED QUALIFIERS**

Qualifiers which may be applied by the laboratory in compliance with applicable requirements are as follows.

Commonly used laboratory metals (inorganic) qualifiers:

- U- Indicates the analyte was analyzed for but not detected in the sample.
- B- Indicates the analyte concentration is less than the CRDL but greater than the IDL.
- E- Indicates the value reported is estimated due to the presence of interference.
- M- Indicates duplicate injection precision criteria were not met during graphite furnace (GFAA) analysis.
- N- Indicates spiked sample recovery was not within the control limits.
- S- Indicates the reported value was determined by the Method of Standard Additions (MSA).
- W- Indicates post-digestion spike for GFAA analysis is outside control limits and the sample absorbance is less than 50% of the spike absorbance.
- \*- Indicates duplicate analysis was not within control limits.
- + - Indicates the correlation coefficient (r) for the MSA was less than 0.995.

## **Qualification Summary Table**

## Qualification Summary Table

## Inorganics (Metals)

ANALYTE	TYPE	QUALIFIER	SAMPLES AFFECTED	DQO	REASON
Thallium	MINOR	UJ	B0GFD7	BLANKS	Preparation blank value is negative and outside acceptance criteria.
Thallium	MINOR	BJ	B0GFD8	BLANKS	Preparation blank value is negative and outside acceptance criteria.
Iron	MINOR	U	B0GFD7	BLANKS	Calibration blank value is positive and outside acceptance criteria.
Silver	MINOR	UJ	B0GFD7 B0GFD8	BLANKS	Preparation blank value is negative and outside acceptance criteria.
Thallium	MINOR	U	B0GFD8	BLANKS	Calibration blank value is positive and outside acceptance criteria.
Aluminum	MINOR	BJ/UJ	B0GFD7 B0GFD8	ACCURACY	No matrix spike analysis completed.
Calcium	MINOR	J	B0GFD7 B0GFD8	ACCURACY	No matrix spike analysis completed.
Iron	MINOR	J/UJ	B0GFD7 B0GFD8	ACCURACY	No matrix spike analysis completed.
Magnesium	MINOR	J	B0GFD7 B0GFD8	ACCURACY	No matrix spike analysis completed.
Potassium	MINOR	J	B0GFD7 B0GFD8	ACCURACY	No matrix spike analysis completed.
Sodium	MINOR	J	B0GFD7 B0GFD8	ACCURACY	No matrix spike analysis completed.
Calcium	MINOR	J	B0GFD8	PRECISION	Serial dilution percent difference is outside acceptance criteria and the sample results are greater than 50 times the instrument detection limit.

## Comments:

1. The field split RPD values will be evaluated in SDG # W0663-QES, LATA ID VB404.07.

## Data Summary Table

9613428.0860

## METALS

## DATA SUMMARY TABLE

LATA ID#: VB404.05		HEIS #:	B0GFD7		B0GFD8	
		Date:	9-Aug-95		9-Aug-95	
		Matrix:	WATER		WATER	
Constituent	CAS #	Units	Results	Q	Results	Q
Aluminum	7429-90-5	ug/L	29.0	UJ	30.3	BJ
Antimony	7440-36-0	ug/L	58.0	U	58.0	U
Arsenic	7440-38-2	ug/L	98.0	U	98.0	U
Barium	7440-39-3	ug/L	146	B	141	B
Beryllium	7440-41-7	ug/L	1.0	U	1.0	U
Cadmium	7440-43-9	ug/L	5.0	U	5.0	U
Calcium	7440-70-2	ug/L	122000	J	124000	J
Chromium	7440-47-3	ug/L	170		158	
Cobalt	7440-48-4	ug/L	6.0	U	6.0	U
Copper	7440-50-8	ug/L	3.0	U	3.0	U
Iron	7439-89-6	ug/L	105	UJ	12.0	UJ
Lead	7439-92-1	ug/L	56.0	U	65.0	B
Magnesium	7439-95-4	ug/L	12400	J	12200	J
Manganese	7439-96-5	ug/L	2.0	U	2.0	U
Nickel	7440-02-0	ug/L	15.0	U	15.0	U
Potassium	7440-09-7	ug/L	7850	J	7580	J
Selenium	7782-49-2	ug/L	87.0	U	87.0	U
Silver	7440-22-4	ug/L	4.0	UJ	4.0	UJ
Sodium	7440-23-5	ug/L	8220	J	7800	J
Thallium	7440-28-0	ug/L	50.0	UJ	109	UJ
Vanadium	7440-62-2	ug/L	4.0	U	5.3	B
Zinc	7440-66-6	ug/L	7.8	B	8.7	B

Shaded areas indicate changes by the validator.

11/21/95, 1:04 PM

40405DST.XLS, METALS

000010

9613428.0861

## Sample Results (Form I's)



9613428.0863

SW - 846

1  
INORGANIC ANALYSES DATA SHEET

CLIENT ID NO.

B0GFD8

Lab Name: L.A.S \_\_\_\_\_ Contract: HANFORD \_\_\_\_\_

Lab Code: LOCK \_\_\_\_\_ Case No.: B95-06 SAS No.: \_\_\_\_\_ SDG No.: L5106F

Matrix (soil/water): WATER Lab Sample ID: L5106-13 \_\_\_\_\_

Level (low/med): LOW \_\_\_\_\_ Date Received: 08/11/95

% Solids: \_\_\_\_\_ 0

Concentration Units (ug/L or mg/kg dry weight): UG/L \_\_\_\_\_

CAS No.	Analyte	Concentration	C	Q	M
7429-90-5	Aluminum	30.3	B		P
7440-36-0	Antimony	58.0	U		P
7440-38-2	Arsenic	98.0	U		P
7440-39-3	Barium	141	B		P
7440-41-7	Beryllium	1.0	U		P
7440-43-9	Cadmium	5.0	U		P
7440-70-2	Calcium	124000	-	E	P
7440-47-3	Chromium	158			P
7440-48-4	Cobalt	6.0	U		P
7440-50-8	Copper	3.0	U		P
7439-89-6	Iron	12.0	U		P
7439-92-1	Lead	65.0	B		P
7439-95-4	Magnesium	12200			P
7439-96-5	Manganese	2.0	U		P
7440-02-0	Nickel	15.0	U		P
7440-09-7	Potassium	7580			P
7782-49-2	Selenium	87.0	U		P
7440-22-4	Silver	4.0	U		P
7440-23-5	Sodium	7800			P
7440-28-0	Thallium	109	B		P
7440-62-2	Vanadium	5.3	B		P
7440-66-6	Zinc	8.7	B		P

BS

J

UJ

J

J

UJ

UJ

BM  
11-9-95

Color Before: \_\_\_\_\_ Clarity Before: \_\_\_\_\_ Texture: \_\_\_\_\_

Color After: \_\_\_\_\_ Clarity After: \_\_\_\_\_ Artifacts: \_\_\_\_\_

Comments:

\_\_\_\_\_  
\_\_\_\_\_  
\_\_\_\_\_

FORM I - IN

000013

BS  
11-2-95

0240

9613428.0864

# Checklist

9613428.0865

LATA INORGANIC (METALS)  
DATA VALIDATION CHECKLIST

VALIDATION LEVEL:	A	B	C	D	E
VALIDATION PROCEDURE:	<input type="checkbox"/> WHC-CM-5-3, Rev. 0		<input checked="" type="checkbox"/> WHC-SD-EN-SPP-002, Rev. 2		
PROJECT:	100-HR-3 ROUND 9		SDG:	LK5106-LAS	
VALIDATOR:	D.E. STROUP	LATA NO:	VB404.05	DATE:	27-Oct-95
REVIEWER:	B MORRIS	LAB:	LAS	CASE:	N/A
SAF NO:	B95-068	QAPP NO:	DOE/RL-88-36, Rev. 0	SAP NO:	N/A
<b>ANALYSES REQUESTED</b>					
<input checked="" type="checkbox"/>	ICP Metals Unfiltered 6010	<input checked="" type="checkbox"/>	ICP Metals Filtered 6010	COMMENTS	
SAMPLE NO.	MATRIX	SAMPLE NO.	MATRIX		
B0GFD7	WATER	B0GFD8	WATER		

1. DATA PACKAGE COMPLETENESS AND CASE NARRATIVE

YES NO N/A

Is technical verification documentation present?

Is a case narrative present?

2. HOLDING TIMES

YES NO N/A

Are sample holding times acceptable?

See HOLDING TIME SUMMARY form

3. INSTRUMENT PERFORMANCE AND CALIBRATIONS

YES NO N/A

Were initial calibrations performed on all instruments?

Are initial calibrations acceptable?

Are ICP interference checks acceptable?

Were ICV and CCV checks performed on all instruments?

Are ICV and CCV checks acceptable?

Validation calculation checks were performed and are acceptable.

If NO(s) are checked, see CALIBRATION DATA SUMMARY form

9613428.0866

LATA INORGANIC (METALS)  
DATA VALIDATION CHECKLIST

4. BLANKS

YES NO N/A

Were ICB and CCB checks performed for all applicable analyses?

Are ICB and CCB results acceptable?

Were preparation blanks analyzed?

Are preparation blank results acceptable?

If NO(s) are checked, see BLANK AND SAMPLE DATA SUMMARY form

5. ACCURACY

YES NO N/A

Were spike samples analyzed at the proper frequency?

Are all spike sample recoveries acceptable?

Are all elements spiked at an appropriate level?

Was a post digestion spike analyzed?

Are all post digestion spike recoveries acceptable?

Were laboratory control samples (LCS) analyzed at the proper frequency?

Are all LCS recoveries acceptable?

Validation calculation checks were performed and are acceptable.

If NO(s) are checked, see ACCURACY DATA SUMMARY form

6. PRECISION

YES NO N/A

Were laboratory duplicates analyzed at the proper frequency?

Are all duplicate RPD values acceptable?

Were MS/MSDs analyzed?

Are all MS/MSD RPD values acceptable?

Were ICP serial dilution samples analyzed at the proper frequency?

Are all ICP serial dilution %D values acceptable?

Validation calculation checks were performed and are acceptable.

If NO(s) are checked, see PRECISION DATA SUMMARY form

9613428-0867

**LATA INORGANIC (METALS)  
DATA VALIDATION CHECKLIST**

**7. FIELD QC SAMPLES**

YES NO N/A

Were field QC samples (field/trip blanks, duplicates, splits, performance audit) identified?

Are field/trip blank results acceptable? (see Blank Data Summary form)

Are field duplicate RPD values acceptable? (see Field QC evaluation)

Are field split RPD values acceptable? (see Field QC evaluation)

Are performance audit sample results acceptable?

**Comments:**

Split analysis results reported in SDG W0663-QES (VB404.07).

**8. FURNACE AA QUALITY CONTROL**

YES NO N/A

Were duplicate injections required?

Are all duplicate injection %RSD values acceptable?

Were analytical spikes required?

Are all analytical spike recoveries acceptable?

Was MSA required?

Are all MSA results acceptable?

Validation calculation checks were performed and are acceptable.

**Comments:**

**9. REPORTED RESULTS AND DETECTION LIMITS**

YES NO N/A

Are results reported for all requested analyses?

Are all results supported in the raw data?

Are results calculated properly?

Do results meet the CRDLs?

Validation calculation checks were performed and are acceptable.

**Comments:**

**VALIDATION SUMMARY**

For deficiencies (major and minor) and comments, please refer to the Qualification Summary Table.

9613428.0868

DATA INORGANIC (METALS)  
DATA VALIDATION CHECKLIST

## HOLDING TIME SUMMARY

SDG: LK5106-LAS			VALIDATOR: D.E. STROUP					DATE: 27-Oct-95		
PROJECT: 100-HR-3 ROUND 9			REVIEWER: B MORRIS					LATA NO.: VB404.05		
HEIS-SN	MATRIX CODE	ANALYSIS	DATE COLLECTED	PREP DATE	ANALYSIS DATE	PREP HT (days)	Required HT (days)	ANALYSIS HT (days)	Required HT (days)	VAL Q
BOGFD7	WATER	ICP Metals - Filtered	9-Aug-95	N/A	30-Aug-95	N/A	N/A	21	180	NONE
BOGFD8	WATER	ICP Metals - Unfiltered	9-Aug-95	N/A	25-Aug-95	N/A	N/A	16	180	NONE

000018

9613428.0869

DATA INORGANIC (METALS)  
DATA VALIDATION CHECKLIST

## BLANK DATA SUMMARY

SDG: LK5106-LAS			VALIDATOR: D.E. STROUP						DATE: 27-Oct-95	
PROJECT: 100-HR-3 ROUND 9			REVIEWER: B MORRIS						LATA NO.: VB404.05	
BLANK ID	ANALYTE	RESULT	LAB Q	RT	UNITS	2X RESULT	5X RESULT	10X RESULT	SAMPLES AFFECTED	VAL Q
Prep Blank	Thallium	-60.770	B	NA	ug/L			607.7	B0GFD7 B0GFD8	BJ/UJ
Cal Blank	Iron	25.3	B	NA	ug/L		126.5		B0GFD7	U
Prep Blank	Silver	-5.290	B	NA	ug/L			52.9	B0GFD7 B0GFD8	UJ
Cal Blank	Thallium	64.4	B	NA	ug/L		322		B0GFD8	U

9613428.0870

SW - 846

3  
BLANKS

Lab Name: L.A.S \_\_\_\_\_

Contract: HANFORD \_\_\_\_\_

Lab Code: LOCK \_\_\_\_\_

Case No.: B95-06

SAS No.: \_\_\_\_\_

SDG No.: L5106F

Preparation Blank Matrix (soil/water): WATER

Preparation Blank Concentration Units (ug/L or mg/kg): UG/L \_\_\_\_\_

Analyte	Initial Calib. Blank (ug/L)		Continuing Calibration Blank (ug/L)						Preparation Blank		M
	C		1	C	2	C	3	C	C		
Aluminum	29.0	U	29.0	U	29.0	U	29.0	U	29.000	U	P
Antimony	58.0	U	58.0	U	58.0	U	58.0	U	58.000	U	P
Arsenic	98.0	U	98.0	U	98.0	U	98.0	U	98.000	U	P
Barium	21.0	U	21.0	U	21.0	U	21.0	U	21.000	U	P
Beryllium	1.0	U	1.0	U	1.0	U	1.0	U	1.000	U	P
Cadmium	5.0	U	5.0	U	5.0	U	5.0	U	5.000	U	P
Calcium	32.0	U	32.0	U	32.0	U	32.0	U	32.000	U	P
Chromium	3.0	U	3.0	U	3.0	U	3.0	U	3.000	U	P
Cobalt	6.0	U	6.0	U	6.0	U	6.0	U	6.000	U	P
Copper	3.0	U	3.0	U	3.0	U	3.0	U	3.000	U	P
Iron	12.0	U	12.0	U	12.0	U	12.0	U	12.000	U	P
Lead	56.0	U	56.0	U	56.0	U	56.0	U	56.000	U	P
Magnesium	50.0	U	50.0	U	50.0	U	50.0	U	50.000	U	P
Manganese	2.0	U	2.0	U	2.0	U	2.0	U	2.000	U	P
Nickel	15.0	U	15.0	U	15.0	U	15.0	U	15.000	U	P
Potassium	600.0	U	600.0	U	600.0	U	600.0	U	600.000	U	P
Selenium	87.0	U	87.0	U	87.0	U	87.0	U	87.000	U	P
Silver	4.0	U	4.0	U	4.0	U	4.0	U	-5.290	B	P
Sodium	70.0	U	70.0	U	70.0	U	70.0	U	70.000	U	P
Thallium	50.0	U	50.0	U	55.9	B	64.4	B	50.000	U	P
Vanadium	4.0	U	4.0	U	4.0	U	4.0	U	4.000	U	P
Zinc	4.0	U	4.0	U	4.0	U	4.0	U	4.000	U	P

FORM III - IN

bis  
11-2-95  
0245

000020

9613428.0871

SW - 846

3  
BLANKS

Lab Name: L.A.S \_\_\_\_\_ Contract: HANFORD \_\_\_\_\_

Lab Code: LOCK \_\_\_\_\_ Case No.: B95-06 SAS No.: \_\_\_\_\_ SDG No.: L5106W

Preparation Blank Matrix (soil/water): WATER

Preparation Blank Concentration Units (ug/L or mg/kg): UG/L\_

Analyte	Initial Calib. Blank (ug/L)	C	Continuing Calibration Blank (ug/L)						Prepa- ration Blank		M
			1	C	2	C	3	C	C		
Aluminum	29.0	U	29.0	U	29.0	U	29.0	U	29.000	U	P
Antimony	58.0	U	58.0	U	58.0	U	58.0	U	58.000	U	P
Arsenic	98.0	U	98.0	U	98.0	U	98.0	U	98.000	U	P
Barium	21.0	U	21.0	U	21.0	U	21.0	U	21.000	U	P
Beryllium	1.0	U	1.0	U	1.0	U	1.0	U	1.000	U	P
Cadmium	5.0	U	5.0	U	5.0	U	5.0	U	5.000	U	P
Calcium	32.0	U	32.0	U	32.0	U	32.0	U	32.000	U	P
Chromium	3.0	U	3.0	U	5.4	B	8.2	B	3.000	U	P
Cobalt	6.0	U	6.0	U	6.0	U	7.5	B	6.000	U	P
Copper	3.0	U	3.0	U	3.0	U	7.9	B	3.000	U	P
Iron	12.0	U	12.0	U	13.8	B	25.3	B	12.000	U	P
Lead	56.0	U	56.0	U	56.0	U	56.0	U	56.000	U	P
Magnesium	50.0	U	50.0	U	50.0	U	50.0	U	50.000	U	P
Manganese	2.0	U	2.0	U	2.5	B	7.0	B	2.000	U	P
Nickel	15.0	U	15.0	U	15.0	U	15.0	U	15.000	U	P
Potassium	600.0	U	600.0	U	600.0	U	600.0	U	600.000	U	P
Selenium	87.0	U	87.0	U	87.0	U	87.0	U	87.000	U	P
Silver	4.0	U	4.0	U	4.0	U	4.0	U	4.000	U	P
Sodium	70.0	U	70.0	U	70.0	U	70.0	U	71.010	B	P
Thallium	-71.3	B	50.0	U	-100.8	B	-149.9	B	-60.770	B	P
Vanadium	4.0	U	4.0	U	4.0	U	8.9	B	4.000	U	P
Zinc	4.0	U	4.0	U	4.0	U	5.1	B	7.290	B	P

FORM III - IN

000021

bis  
11-2-95  
0222

9613428.0872

LATA INORGANIC (METALS)  
DATA VALIDATION CHECKLIST

ACCURACY DATA SUMMARY

SDG: LK5106-LAS		VALIDATOR: D.E. STROUP			DATE: 27-Oct-95					
PROJECT: 100-HR-3 ROUND 9		REVIEWER: B MORRIS			LATA NO.: VB404.05					
HEIS-SN	ANALYTE	Lab Q	Actual Spiking Level	Minimum Required Spiking Level	Difference	PERCENT RECOVERY (%R)			SAMPLES AFFECTED	VAL Q
						Matrix Spike	Matrix Spike Duplicate	Laboratory Control Standard		
B0GFD7 B0GFD8	Aluminum					NO MATRIX SPIKE ANALYSIS			B0GFD7/B0GFD8	UJ/BJ
B0GFD7 B0GFD8	Calcium					NO MATRIX SPIKE ANALYSIS			B0GFD7/B0GFD8	J
B0GFD7 B0GFD8	Iron					NO MATRIX SPIKE ANALYSIS			B0GFD7/B0GFD8	J/UJ
B0GFD7 B0GFD8	Magnesium					NO MATRIX SPIKE ANALYSIS			B0GFD7/B0GFD8	J
B0GFD7 B0GFD8	Potassium					NO MATRIX SPIKE ANALYSIS			B0GFD7/B0GFD8	J
B0GFD7 B0GFD8	Sodium					NO MATRIX SPIKE ANALYSIS			B0GFD7/B0GFD8	J

9613428.0873

SW - 846

5A  
SPIKE SAMPLE RECOVERY

CLIENT ID NO.

B0GFD7S

Lab Name: L.A.S \_\_\_\_\_

Contract: HANFORD \_\_\_\_\_

Lab Code: LOCK\_\_

Case No.: B95-06

SAS No.: \_\_\_\_\_

SDG No.: L5106W

Matrix (soil/water): WATER\_\_

Level (low/med): LOW\_\_

% Solids for Sample: \_\_0.0

Concentration Units (ug/L or mg/kg dry weight): UG/L\_\_

Analyte	Control Limit %R	Spiked Sample Result (SSR) C	Sample Result (SR) C	Spike Added (SA)	%R	Q	M
Aluminum							NR
Antimony	75-125	2049.4400	58.0000 U	2000.00	102.5		P
Arsenic	75-125	2122.7300	98.0000 U	2000.00	106.1		P
Barium	75-125	2186.7600	145.8600 B	2000.00	102.0		P
Beryllium	75-125	46.6200	1.0000 U	50.00	93.2		P
Cadmium	75-125	48.4200	5.0000 U	50.00	96.8		P
Calcium							NR
Chromium	75-125	377.1800	169.6500	200.00	103.8		P
Cobalt	75-125	514.9600	6.0000 U	500.00	103.0		P
Copper	75-125	257.4300	3.0000 U	250.00	103.0		P
Iron							NR
Lead	75-125	540.7700	56.0000 U	500.00	108.2		P
Magnesium							NR
Manganese	75-125	523.0300	2.0000 U	500.00	104.6		P
Nickel	75-125	533.6500	15.0000 U	500.00	106.7		P
Potassium							NR
Selenium	75-125	2149.0300	87.0000 U	2000.00	107.5		P
Silver	75-125	50.9100	4.0000 U	50.00	101.8		P
Sodium							NR
Thallium	75-125	1843.2200	50.0000 U	2000.00	92.2		P
Vanadium	75-125	525.9500	4.0000 U	500.00	105.2		P
Zinc	75-125	543.1400	7.7500 B	500.00	107.1		P

Comments:

---



---



---

FORM V (Part 1) - IN

*10-19-95*

000023 0225

9613428.0874

SW - 846

5A  
SPIKE SAMPLE RECOVERY

CLIENT ID NO.

B0GFD8S

Lab Name: L.A.S

Contract: HANFORD

Lab Code: LOCK

Case No.: B95-06

SAS No.:

SDG No.: L5106F

Matrix (soil/water): WATER

Level (low/med): LOW

% Solids for Sample: 0.0

Concentration Units (ug/L or mg/kg dry weight): UG/L

Analyte	Control Limit %R	Spiked Sample Result (SSR) C	Sample Result (SR) C	Spike Added (SA)	%R	Q	M
Aluminum							NR
Antimony	75-125	2032.9800	58.0000 U	2000.00	101.6		P
Arsenic	75-125	2180.2300	98.0000 U	2000.00	109.0		P
Barium	75-125	2213.3500	141.1500 B	2000.00	103.6		P
Beryllium	75-125	47.8400	1.0000 U	50.00	95.7		P
Cadmium	75-125	47.2900	5.0000 U	50.00	94.6		P
Calcium							NR
Chromium	75-125	373.1900	158.1700	200.00	107.5		P
Cobalt	75-125	531.6500	6.0000 U	500.00	106.3		P
Copper	75-125	252.6500	3.0000 U	250.00	101.1		P
Iron							NR
Lead	75-125	528.2700	65.0100 B	500.00	92.7		P
Magnesium							NR
Manganese	75-125	528.9500	2.0000 U	500.00	105.8		P
Nickel	75-125	535.1800	15.0000 U	500.00	107.0		P
Potassium							NR
Selenium	75-125	2233.3600	87.0000 U	2000.00	111.7		P
Silver	75-125	50.8900	4.0000 U	50.00	101.8		P
Sodium							NR
Thallium	75-125	2076.5200	109.4400 B	2000.00	98.4		P
Vanadium	75-125	532.8000	5.3400 B	500.00	105.5		P
Zinc	75-125	541.7800	8.7400 B	500.00	106.6		P

Comments:

---



---



---

FORM V (Part 1) - IN

*10-19-95*

000024

0248

9613428.0875

LATA INORGANIC (METALS)  
DATA VALIDATION CHECKLIST

PRECISION DATA SUMMARY

SDG: LK5106-LAS			VALIDATOR: D.E. STROUP										DATE: 27-Oct-95		
PROJECT: 100-HR-3 ROUND 9			REVIEWER: B MORRIS										LATA NO.: VB404.05		
HEIS-SN	ANALYTE	RESULTS	LAB Q	IDL µg/L	10*IDL µg/L	50*IDL µg/L	SERIAL DIL %D	CRDL µg/L	2 CRDL mg/Kg	5 CRDL mg/Kg	DUPE RPD %	DUPE CRDL dif	MS/MSD RPD	SAMPLES AFFECTED	VAL Q
B0GFD8L	Calcium	124000		32	NA	1600	10.7%	5000	NA	NA	NA	NA	NA	B0GFD8	J

000025

9613428.0876

SW - 846

9  
ICP SERIAL DILUTION

CLIENT ID NO.

BOGFD8 L

Lab Name: L.A.S \_\_\_\_\_ Contract: HANFORD \_\_\_\_\_

Lab Code: LOCK \_\_\_\_\_ Case No.: B95-06 SAS No.: \_\_\_\_\_ SDG No.: L5106F

Matrix (soil/water): WATER Level (low/med): LOW \_\_\_\_\_

Concentration Units: ug/L

Analyte	Initial Sample Result (I)	C	Serial Dilution Result (S)	C	% Difference	Q	M
Aluminum	30.31	B	145.00	U	100.0	-	P
Antimony	58.00	U	290.00	U		-	P
Arsenic	98.00	U	490.00	U		-	P
Barium	141.15	B	139.93	B	0.9	-	P
Beryllium	1.00	U	5.00	U		-	P
Cadmium	5.00	U	25.00	U		-	P
Calcium	124216.59	-	110899.94	-	10.7	E	P
Chromium	158.17	-	148.13	-	6.3	-	P
Cobalt	6.00	U	30.00	U		-	P
Copper	3.00	U	15.00	U		-	P
Iron	12.00	U	60.00	U		-	P
Lead	65.01	B	280.00	U	100.0	-	P
Magnesium	12164.32	-	11577.05	B	4.8	-	P
Manganese	2.00	U	10.00	U		-	P
Nickel	15.00	U	75.00	U		-	P
Potassium	7581.24	-	5379.88	B	29.0	-	P
Selenium	87.00	U	435.00	U		-	P
Silver	4.00	U	20.00	U		-	P
Sodium	7803.88	-	7783.74	B	0.3	-	P
Thallium	109.44	B	250.00	U	100.0	-	P
Vanadium	5.34	B	20.00	U	100.0	-	P
Zinc	8.74	B	26.88	B	207.6	-	P

FORM IX - INL

BAM  
11-9-95

000026

0251

9613428.0877

LATA INORGANIC (METALS)  
DATA VALIDATION CHECKLIST

PERCENT RECOVERY (ICV/CCV)

SDG: LK5106-LAS

Date: 27-Oct-95

LATA No.: VB404.05

Validator: D.E. STROUP

Analyte	ICV/CCV ID	Observed Value	True Value	%R
		O	A	
Calcium (BOGFD7)	ICV	102257.50	100000.00	102.3%
Zinc (BOGFD7)	ICV	10030.22	10000.00	100.3%
Calcium (BOGFD7)	CCV2	26569.31	25000.00	106.3%
Zinc (BOGFD7)	CCV2	10688.70	10000.00	106.9%
Calcium (BOGFD8)	ICV	103171.80	100000.00	103.2%
Zinc (BOGFD8)	ICV	9951.67	10000.00	99.5%
Calcium (BOGFD8)	CCV2	25108.09	25000.00	100.4%
Zinc (BOGFD8)	CCV2	10139.25	10000.00	101.4%

000027

9613428.0878

LATA INORGANIC (METALS)  
DATA VALIDATION CHECKLIST

MATRIX SPIKE RECOVERY (MS)

SDG: LK5106-LASDate: 27-Oct-95LATA No.: VB404.05Validator: D.E. STROUP

Analyte	Sample ID	Spike Sample	Sample	Spike	%R
		Result	Result	Added	
		SSR	SR	SA	
<u>Antimony</u>	<u>B0GFD7S</u>	<u>2049.44</u>	<u>0.00</u>	<u>2000.00</u>	<u>102.5%</u>
<u>Cobalt</u>	<u>B0GFD7S</u>	<u>514.96</u>	<u>0.00</u>	<u>500.00</u>	<u>103.0%</u>
<u>Antimony</u>	<u>B0GFD8S</u>	<u>2032.98</u>	<u>0.00</u>	<u>2000.00</u>	<u>101.6%</u>
<u>Cobalt</u>	<u>B0GFD8S</u>	<u>531.65</u>	<u>0.00</u>	<u>500.00</u>	<u>106.3%</u>

000028

9613428.0879

LATA INORGANIC (METALS)  
DATA VALIDATION CHECKLIST

PERCENT RECOVERY (LCS)

SDG: LK5106-LAS

Date: 27-Oct-95

LATA No.: VB404.05

Validator: D.E. STROUP

Analyte	Observed value	True value	%R
	OLCS	ALCS	
Aluminum	1971.15	2000.00	98.6%
Silver	45.51	50.00	91.0%

000029

9613428.0850

LATA INORGANIC (METALS)  
DATA VALIDATION CHECKLIST

RELATIVE PERCENT DIFFERENCE

SDG: LK5106-LAS

Date: 27-Oct-95

LATA No.: VB404.05

Validator: D.E. STROUP

Analyte	Sample ID	Original (Sample)	Duplicate	RPD
		concentration	concentration	
		OS	D	
Barium	B0GFD7D	145.86	145.65	0.1%
Zinc	B0GFD7D	7.75	12.42	46.3%
Barium	B0GFD8D	141.15	142.52	1.0%
Zinc	B0GFD8D	8.74	9.02	3.2%

9613429.0881

LATA INORGANIC (METALS)  
DATA VALIDATION CHECKLIST

PERCENT DIFFERENCE (ICP SERIAL DILUTION)

SDG: LK5106-LAS

Date: 27-Oct-95

LATA No.: VB404.05

Validator: D.E. STROUP

Analyte	Analyte Concentration before Dilution	Analyte Concentration after Serial Dilution	%D
	I	S	
<u>Barium (B0GFD7L)</u>	<u>145.86</u>	<u>146.02</u>	0.1%
<u>Chromium (B0GFD7L)</u>	<u>169.65</u>	<u>173.98</u>	2.6%
<u>Barium (B0GFD8L)</u>	<u>141.15</u>	<u>139.93</u>	0.9%
<u>Chromium (B0GFD8L)</u>	<u>158.17</u>	<u>148.13</u>	6.3%

**000031**

9613428.0882

LATA INORGANIC (METALS)  
DATA VALIDATION CHECKLIST

INORGANICS RESULTS CALCULATION, WATER

SDG: LK5106-LAS

Date: 27-Oct-95

LATA No.: VB404.05

Validator: D.E. STROUP

Analyte	Concentration from curve		Dilution Factor	Concentration (µg/L)
	CONCW	units		
<u>Calcium (B0GFD7)</u>	<u>122000.00</u>	<u>ug/L</u>	<u>1</u>	122000.0
<u>Potassium (B0GFD7)</u>	<u>7845.00</u>	<u>ug/L</u>	<u>1</u>	7845.0
<u>Calcium (B0GFD8)</u>	<u>124000.00</u>	<u>ug/L</u>	<u>1</u>	124000.0
<u>Lead (B0GFD8)</u>	<u>65.00</u>	<u>ug/L</u>	<u>1</u>	65.0

000032

9613428.0883

## Laboratory Case Narrative

Lockheed Analytical Services

Log-in No.: L5106  
Quotation No.: Q400000-B  
SAF: B95-068  
Document File No.: 0811596  
WHC Document File No.: 257  
SDG No.: LK5106  
Page 3

## CASE NARRATIVE INORGANIC METALS ANALYSES

The routine calibration and quality control analyses performed for this batch include as applicable: instrument tune (ICP/MS only), initial and continuing calibration verification, initial and continuing calibration blanks, method blank(s), laboratory control sample(s), ICP interference check samples (ICP only), serial dilutions, analytical (post-digestion) spike samples, matrix spike (predigestion) sample(s), duplicate sample(s).

### Preparation and Analysis Requirements

- One water sample for total metals analysis. The sample was prepared as LAS Batch 811BHT and analyzed for selected analytes as requested on the chain of custody. Sample B0GFD7 (L5106-2) was used for matrix spike and duplicate and serial dilution. All data flags due to the performance of the above-mentioned QC are also associated with every sample digested with this batch.

### Holding Time Requirements

- All samples were analyzed within the method-specific holding times.

### Internal Quality Control

- All internal quality control were within acceptance limits with the following exceptions:  
For lead, the LCSW (121.1%) recovered slightly above the acceptance criteria (80-120%). No lead was detected in the sample, therefore the positive bias observed does not affect the result. No corrective action was taken.

### Sample Results

- The following qualifiers are reported on the basis of the techniques employed to perform the analyses:

"P" ICP-AES

Nalini Prabhakar

09/08/95

Prepared By

Date

*28* 10-27-95

~~0007~~

**000034**

Lockheed Analytical Services

Log-in No.: L5106  
 Quotation No.: Q400000-B  
 SAF: B95-068  
 Document File No.: 0811596  
 WHC Document File No.: 257  
 SDG No.: LK5106  
 Page 4

## CASE NARRATIVE INORGANIC METALS ANALYSES

The routine calibration and quality control analyses performed for this batch include as applicable: instrument tune (ICP/MS only), initial and continuing calibration verification, initial and continuing calibration blanks, method blank(s), laboratory control sample(s), ICP interference check samples (ICP only), serial dilutions, analytical (post-digestion) spike samples, matrix spike (predigestion) sample(s), duplicate sample(s).

### Preparation and Analysis Requirements

- One filtered water sample was analyzed for dissolved metals analysis. As the measured turbidity of the sample was less than 1 NTU, it was batched as LAS batch 811BHD for dissolved metals analysis. Sample BOGFD8 (L5106-13) was used for matrix spike, duplicate and serial dilution analyses. All data flags due to the performance of the above-mentioned QC sample are also associated with every sample analyzed with this batch.

### Holding Time Requirements

- All samples were analyzed within the method-specific holding times.

### Method Blanks

- The level of analytes in the method blanks were less than the reporting detection limits.

### Internal Quality Control

All internal quality control were within acceptance limits with the following exceptions:

- In the analysis of calcium, the percent difference of serial dilution slightly exceeded 10% the control limit. This may be due to physical interferences. Calcium results for the associated sample is flagged with an "E".

### Sample Results

- The following qualifiers are reported on the basis of the techniques employed to perform the analyses:  
 "P" ICP-AES

Nalini Prabhakar  
 Prepared By

09/08/95

Date

*10-27-95*

*0008*

**000035**

9613428.0886

## **Chain-of-Custody Information**

Bechtel Hanford, Inc.

# L5106 CHAIN OF CUSTODY/SAMPLE ANALYSIS REQUEST

Data Turnaround  
 Priority  
 Normal

Collector <i>K.D Lee</i>	Company Contact R. E. Peterson	Telephone (509) 372-9638
Project Designation 100-HR-3 Groundwater Sampling, Round 9, Phase 2	Sampling Location 100 D	SAF No. B95-068
Ice Chest No. <i>Patton</i>	Field Logbook No. <i>E.F.L. - 1018</i>	Method of Shipment Federal Express
Shipped To Lockheed	Offsite Property No. <i>NA-2-10-95 W95-0-0204-46</i>	Bill of Lading/Air Bill No. <i>2904637303</i>

Possible Sample Hazards/Remarks	Preservation	HNO <sub>3</sub>	Cool 4°C	H <sub>2</sub> SO <sub>4</sub>	*1	H <sub>2</sub> SO <sub>4</sub>	HNO <sub>3</sub>	Cool 4°C	Cool 4°C		HNO <sub>3</sub>
	Type of Container	G	G	P/G	P	P/G	P/G	G	P/G		G
	No. of Container(s)	1	1	1	1	1	5	1	1		1
Special Handling and/or Storage Maintain samples between 2°C and 6°C.	Volume	500mL	500mL	500mL	1L	1L	1L	500mL	20mL		500mL
SAMPLE ANALYSIS	ICP Metals (Unfiltered)	Anions (IC) - F, Cl, SO <sub>4</sub> , NO <sub>2</sub> , NO <sub>3</sub> , PO <sub>4</sub>	NO <sub>2</sub> - NO <sub>3</sub>	Sulfide	Ammonia	Gross Alpha, Gross Beta, Sr-90	Tritium	Activity Scan			ICP Metals (Filtered)

Sample No.	Matrix*	Date Sampled	Time Sampled									
BOGFD7	W	8/9/95	1135	X	X	X	X	X	X	X		
BOGFD8	W	8/9/95	1135									X

CHAIN OF POSSESSION		Sign/Print Names		SPECIAL INSTRUCTIONS				Matrix*	
Relinquished By <i>K.D Lee</i> Date/Time <i>8/10/95 0730</i>		Received By <i>B. Whitten</i> Date/Time <i>8-10-95</i>		*1 ZnAc + NaOH  Sample analysis for phosphate, nitrate, and nitrite by EPA 300.0; and turbidity by EPA 180.1 is being requested for information only. The ERC Contractor acknowledges that the 48-hour holding time will not be met.  The Activity Scan is for all samples listed on this chain of custody.				<ul style="list-style-type: none"> <li>S - Soil</li> <li>SE - Sediment</li> <li>SO - Solid</li> <li>SL - Sludge</li> <li>W - Water</li> <li>O - Oil</li> <li>A - Air</li> <li>DS - Drum Solids</li> <li>DL - Drum Liquids</li> <li>T - Tissue</li> <li>WI - Wipe</li> <li>L - Liquid</li> <li>V - Vegetation</li> <li>X - Other</li> </ul>	
Relinquished By <i>B. Whitten</i> Date/Time <i>8-10-95</i>		Received By _____ Date/Time _____							
Relinquished By _____ Date/Time _____		Received By _____ Date/Time _____							
Relinquished By _____ Date/Time _____		Received By _____ Date/Time _____							
LABORATORY SECTION	Received By <i>AMM</i>	Title <i>Complete Custodian</i>	Date/Time <i>8-11-95 0700</i>						
FINAL SAMPLE DISPOSITION	Disposal Method _____		Disposed By _____	Date/Time _____					

8/10-01-27-95  
 19115476

430000

9613428.0888

**END OF PACKAGE**

**DATA VALIDATION REPORT**  
**for**  
**100-HR-3 GROUNDWATER ROUND 9**  
**PHASE II**  
**General Chemistry Analysis**  
**SDG LK5106-LAS**  
**LATA VB404.05**

Bechtel Hanford Inc.  
P.O. Box 969  
Richland, Washington

November 10, 1995

## Table of Contents

Data Validation Narrative .....	000002
INTRODUCTION .....	000002
ANALYSES REQUESTED .....	000002
DATA QUALITY OBJECTIVES .....	000002
REFERENCES .....	000004
GLOSSARY OF VALIDATION APPLIED QUALIFIERS (CHEMISTRY) .....	000005
GLOSSARY OF LABORATORY APPLIED QUALIFIERS .....	000006
Qualification Summary Table .....	000007
Data Summary Table .....	000009
Sample Results .....	000011
Checklist .....	000013
Laboratory Case Narrative .....	000027
Chain-of-Custody Information .....	000029
Supplemental Information .....	000031
END OF PACKAGE .....	000035

**100-HR-3 GROUNDWATER ROUND 9 PHASE II  
Data Validation Narrative**

**INTRODUCTION**

All samples in Sample Delivery Group (SDG) LK5106-LAS (VB404.04) were validated at level D as defined in the Data Validation Procedures for Chemical Analysis (WHC-SD-EN-SPP-002, Rev. 2).

The analyses were performed by Lockheed Analytical Services.

**ANALYSES REQUESTED**

See Table 1:

**DATA QUALITY OBJECTIVES**

- Precision:** Goals for precision were met.
- Accuracy:** Goals for accuracy were met with the exception of those items discussed in the "**Qualification Summary Table**".
- Sample Result Verification:** All sample results were supported in the raw data.
- Detection Limits:** Detection limit goals were met for all sample results as specified in the *RCRA Facility Investigation/Corrective Measures Study Plan for the 100-HR-3 Operable Unit*, DOE/RL-88-36, Rev.0.
- Completeness:** The data package was 78% complete for all requested analyses.

**MAJOR DEFICIENCIES**

Major deficiencies were identified during validation which required qualification of data as unusable. See the "**Qualification Summary Table**".

**MINOR DEFICIENCIES**

Minor deficiencies were identified during validation which required qualification of data as estimated. See the "**Qualification Summary Table**".

9613428.0892

**Table 1**  
**Chain-of-Custody**  
**Analysis Request**

LATA ID #: VB404.05

SDG: LK5106-LAS

Sample Information					Analyses Requested			
SAMPLE NO.	DATE COLLECTED	MATRIX	SAF	FIELD QC INFO	1	2	3	4
B0GFD7	9-Aug-95	WATER	B95-068	Split of B0GFB1	X	X	X	X

**Method References:**

<u>Analysis</u>	<u>Method</u>
1. Anions (Cl,F,NO <sub>2</sub> ,NO <sub>3</sub> ,PO <sub>4</sub> ,SO <sub>4</sub> )	300.0
2. Ammonia	350.1
3. NO <sub>2</sub> +NO <sub>3</sub>	353.2
4. Sulfide	9030

**REFERENCES**

WHC 1993, *Data Validation Procedures for Chemical Analyses*, WHC-SD-EN-SPP-002, Rev. 2, Westinghouse Hanford Company, Richland, Washington.

DOE 1992, *RCRA Facility Investigation/Corrective Measures Study Plan for the 100-HR-3 Operable Unit*, DOE/RL-88-36, Rev.0, Department of Energy-Hanford, Richland, Washington.

**GLOSSARY OF VALIDATION APPLIED QUALIFIERS (CHEMISTRY)**

Qualifiers which may be applied by data validators in compliance with the procedures herein are as follows.

- U- Indicates the compound or analyte was analyzed for and not detected in the sample. The value reported is the sample quantitation limit corrected for sample dilution and moisture content by the laboratory.
- UJ- Indicates the compound or analyte was analyzed for and not detected in the sample. Due to a QC deficiency identified during data validation, the associated quantitation limit is an estimate.
- J- Indicates the compound or analyte was analyzed for and detected. The associated concentration is an estimate, but the data are usable for decision making purposes.
- BJ- Applied to inorganic analyses only. Indicates the analyte concentration was greater than the IDL but less than the CRDL and is considered an estimated value.
- R- Indicates the compound or analyte was analyzed for, detected, and due to an identified QC deficiency the data are unusable.
- UR- Indicates the compound or analyte was analyzed for and not detected in the sample. Additionally, the data are unusable due to an identified QC deficiency.

## GLOSSARY OF LABORATORY APPLIED QUALIFIERS

Qualifiers which may be applied by the laboratory in compliance with applicable requirements are as follows.

Commonly used laboratory general chemistry qualifiers:

- U- Indicates the analyte was analyzed for but not detected in the sample.
- H- Sample analysis performed outside of method-or client specified maximum holding time requirement.
- D- Presence of high levels of interfering constituents required dilution of sample which increased the RDL by the dilution factor.
- a- The spike recovery and/or RPD for matrix spike duplicates cannot be evaluated due to insufficient spiking level compared to the elevated sample analyte concentration.

9613428.0896

## **Qualification Summary Table**

## Qualification Summary Table

## General Chemistry

ANALYTE	TYPE	QUALIFIER	SAMPLES AFFECTED	DQO	REASON
Nitrite	MAJOR	UR	B0GFD7	HOLD TIME	Holding time is exceeded by greater than 2 times.
Ortho Phosphate	MAJOR	UR	B0GFD7	HOLD TIME	Holding time is exceeded by greater than 2 times.
Nitrate	MINOR	J	B0GFD7	HOLD TIME	Holding time is exceeded by greater than 2 times.
Sulfide	MINOR	UJ	B0GFD7	ACCURACY	Laboratory control standard recovery is outside acceptance criteria.

**Comments:**

1. The laboratory case narrative stated that all quality control samples results were acceptable, however, the sulfide LCS was outside acceptance limits.
2. The field split RPD values will be evaluated in SDG # W0663-QES, (LATA ID # VB404.07).

**000008**

9613428.0898

## Data Summary Table

9613428.0899

**GENERAL CHEMISTRY  
DATA SUMMARY TABLE**

LATA ID#: VB404.05		HEIS #:	B0GFD7
		Date:	9-Aug-95
		Matrix:	WATER
Constituent	CAS #	Units	Results Q
Chloride by IC	16887-00-6	mg/L	27
Fluoride by IC	16984-48-8	mg/L	0.001 U
Sulfate by IC	14808-79-8	mg/L	130
Nitrate by IC	14797-55-8	mg/L	35 J
Nitrite by IC	14797-655-0	mg/L	0.002 UR
Nitrite+Nitrate	NO <sub>2</sub> +NO <sub>3</sub> -N	mg/L	35
Ortho Phosphate by IC	14265-44-2	mg/L	0.020 UR
Ammonia Nitrogen	7664-41-7	mg/L	0.46
Sulfide	18496-25-8	mg/L	1.0 UJ

000010

9613428.0900

## Sample Results (Form I's)

9613428.0901

LOCKHEED ANALYTICAL SERVICES

Sample Results

Client Sample ID: BOGFD7	Date Collected: 09-AUG-95
Matrix: Water	Date Received: 11-AUG-95
Percent Solids: N/A	

Constituent	Units	Method	Result	Project Reporting Limit	Data Qualifier(s)	Date Analyzed	LAS Batch ID	LAS Sample ID
Chloride	mg/L	300.0	27.	0.020		14-AUG-95	26209	L5106-3
Fluoride	mg/L	300.0	< 0.001	0.10	U	05-SEP-95	26210	L5106-3
Nitrate-N	mg/L	300.0	35.	0.020	# J	14-AUG-95	26211	L5106-3
Nitrite-N	mg/L	300.0	< 0.002	0.010	# UR	14-AUG-95	26212	L5106-3
Ortho Phosphate	mg/L	300.0	< 0.020	0.10	# UR	14-AUG-95	26213	L5106-3
Sulfate	mg/L	300.0	130	0.10		14-AUG-95	26214	L5106-3
Ammonia Nitrogen	mg/L	350.1	0.46	0.050		16-AUG-95	26215	L5106-6
Nitrate-Nitrite-Nitrogen	mg/L	353.2	35.	0.50	D(1:10)	18-AUG-95	26217	L5106-4
Sulfide	mg/L	9030	< 1.0	3.0	# UJ	15-AUG-95	26249	L5106-5

000012

bis  
10-17-95  
~~0023~~

9613428.0902

## Checklist

9613428.0903

LATA GENERAL CHEMISTRY  
DATA VALIDATION CHECKLIST

VALIDATION LEVEL:	A	B	C	D	E
VALIDATION PROCEDURE:	<input type="checkbox"/> WHC-CM-5-3, Rev. 0		<input checked="" type="checkbox"/> WHC-SD-EN-SPP-002, Rev. 2		
PROJECT:	100-HR-3 ROUND 6		SDG:	LK5106-LAS	
VALIDATOR:	BJ SEYMOUR	LATA NO:	VB404.05	DATE:	17-Oct-95
REVIEWER:	BJ MORRIS	LAB:	LAS	CASE:	N/A
SAF NO:	B95-068	QAPP NO:	DOE/RL-88-36, Rev. 0	SAP NO:	N/A
<b>ANALYSES REQUESTED</b>					
<input checked="" type="checkbox"/> Anions 300.0	<input checked="" type="checkbox"/> Ammonia 350.1	<input checked="" type="checkbox"/> Nitrate+Nitrite 353.2	<input checked="" type="checkbox"/> Sulfide 9030		
SAMPLE NO.	MATRIX	COMMENTS:			
B0GFD7	WATER				

**1. DATA PACKAGE COMPLETENESS AND CASE NARRATIVE**

YES NO N/A

Is technical verification documentation present?

Is a case narrative present?

**2. HOLDING TIMES**

YES NO N/A

Are sample holding times acceptable?

See HOLDING TIME SUMMARY form

**3. INSTRUMENT PERFORMANCE AND CALIBRATIONS**

YES NO N/A

Were initial calibrations performed on all instruments?

Are initial calibrations acceptable?

Were calibration checks performed on all instruments?

Are calibration checks acceptable?

Validation calculation checks were performed and are acceptable.

If NO(s) are checked, see CALIBRATION DATA SUMMARY form

9613428.0904

LATA GENERAL CHEMISTRY  
DATA VALIDATION CHECKLIST

## 4. BLANKS

YES NO N/A

Were laboratory blanks performed for all applicable analyses?

Are laboratory blank results acceptable?

Were preparation blanks analyzed?

Are preparation blank results acceptable?

If NO(s) are checked, see BLANK AND SAMPLE DATA SUMMARY form

## 5. ACCURACY

YES NO N/A

Were spike samples analyzed at the proper frequency?

Are all spike sample recoveries acceptable?

Were laboratory control samples (LCS) analyzed at the proper frequency?

Are all LCS recoveries acceptable?

Validation calculation checks were performed and are acceptable.

If NO(s) are checked, see ACCURACY DATA SUMMARY form

## 6. PRECISION

YES NO N/A

Were laboratory duplicates analyzed at the proper frequency?

Are all duplicate RPD values acceptable?

Were MS/MSDs analyzed?

Are all MS/MSD RPD values acceptable?

Validation calculation checks were performed and are acceptable.

If NO(s) are checked, see PRECISION DATA SUMMARY form

## 7. FIELD QC SAMPLES

YES NO N/A

Were field QC samples (field/trip blanks, duplicates, splits, performance audit) identified?

Are field/trip blank results acceptable? (see Blank Data Summary form)

Are field duplicate RPD values acceptable? (see Field QC calculations)

Are field split RPD values acceptable? (see Field QC calculations)

Are performance audit sample results acceptable?

  **Comments:** Sample B0GFD7 is identified as a split of B0GFB1

The split is evaluated in SDG: W0663-QES ( LATA ID 404.07).

9613428.0905

DATA GENERAL CHEMISTRY  
DATA VALIDATION CHECKLIST

8. ANALYTE QUANTITATION

YES NO N/A

Was analyte quantitation performed properly?

Are results calculated properly?

Validation calculation checks were performed and are acceptable.

Comments:

---

---

---

---

---

9. REPORTED RESULTS AND DETECTION LIMITS

YES NO N/A

Are results reported for all requested analyses?

Are all results supported in the raw data?

Do results meet the CRDLs?

Validation calculation checks were performed and are acceptable.

Comments:

---

---

---

---

---

VALIDATION SUMMARY

For deficiencies (major and minor) and comments, please refer to the Qualification Summary Table.

9613428-0906

LATA GENERAL CHEMISTRY  
DATA VALIDATION CHECKLIST

## HOLDING TIME SUMMARY

SDG: LK5106-LAS			VALIDATOR: BJ SEYMOUR					DATE: 17-Oct-95		
PROJECT: 100-HR-3 ROUND 9			REVIEWER: BJ MORRIS					LATA NO.: VB404.05		
HEIS-SN	MATRIX CODE	ANALYSIS	DATE COLLECTED	PREP DATE	ANALYSIS DATE	PREP HT (days)	Required HT (days)	ANALYSIS HT (days)	Required HT (days)	VAL Q
BOGFD7	WATER	Anions(Cl,SO <sub>4</sub> )	9-Aug-95	N/A	14-Aug-95	N/A	N/A	5	28	NONE
BOGFD7	WATER	Fluoride	9-Aug-95	N/A	05-Sep-95	N/A	N/A	27	28	NONE
BOGFD7	WATER	Anions(NO <sub>2</sub> ,NO <sub>3</sub> ,PO <sub>4</sub> )	9-Aug-95	N/A	14-Aug-95	N/A	N/A	5	2	J/UR
BOGFD7	WATER	Ammonia	9-Aug-95	N/A	16-Aug-95	N/A	N/A	7	28	NONE
BOGFD7	WATER	Nitrate+Nitrite	9-Aug-95	N/A	18-Aug-95	N/A	N/A	9	28	NONE
BOGFD7	WATER	Sulfide	9-Aug-95	N/A	15-Aug-95	N/A	N/A	6	7	NONE

000017

9613428.0907

LATA GENERAL CHEMISTRY  
DATA VALIDATION CHECKLIST

## ACCURACY DATA SUMMARY

SDG: LK5106-LAS				VALIDATOR: BJ SEYMOUR		DATE: 17-Oct-95		
PROJECT: 100-HR-3 ROUND 9				REVIEWER: BJ MORRIS		LATA NO.: VB404.05		
				PERCENT RECOVERY (%R)				
HEIS-SN	ANALYTE	RESULTS	Lab Q	Matrix Spike	Matrix Spike Duplicate	Laboratory Control Standard	SAMPLES AFFECTED	VAL Q
B0GFD7	Sulfide	<1.0				71.9%	B0GFD7	UJ

000018

9613428.0908

LOCKHEED ANALYTICAL LABORATORY  
 WATER QUALITY PARAMETERS  
 QUALITY CONTROL DATA SUMMARY

SDG:N/A	ANALYTE: TOTAL SULFIDE
LAL BATCH: 811-bh	UNITS: mg/L

## LABORATORY CONTROL SAMPLES

LCS ID	ACCEPTANCE LIMITS (%R)	TRUE VALUE	FOUND VALUE	% RECOVERY
lcs	70-130	7.96	5.725	71.9

## MATRIX SPIKE SAMPLES

CLIENT SAMPLE ID	ACCEPTANCE LIMITS (%R)	SPIKED SAMPLE RESULT	SAMPLE RESULT	SPIKE ADDED	% RECOVERY
BOGFD7	65-135	7.206	0.600 U	7.960	90.5

## LABORATORY DUPLICATE SAMPLES

CLIENT SAMPLE ID	ACCEPTANCE LIMITS (%RPD)	SAMPLE VALUE	DUPLICATE VALUE	RPD
BOGFD7	20	0.600 U	0.600 U	b

## FIELD DUPLICATE SAMPLES

CLIENT SAMPLE ID	CLIENT DUPLICATE SAMPLE ID	SAMPLE VALUE	DUPLICATE VALUE	RPD
N/A				

## FIELD BLANK SAMPLES

CLIENT SAMPLE ID	ANALYSIS RESULT
N/A	

## MATRIX BLANK SAMPLES

LAL SAMPLE ID	ANALYSIS RESULT
pb	0.600 U

BM  
11-9-95

000019

0052

9613428.0909

**LATA GENERAL CHEMISTRY  
CALCULATION SPREADSHEET**

**LINEAR REGRESSION ANALYSIS**

SDG: LK5106-LASDate: 17-Oct-95LATA No.: VB404.05Validator: BJ SEYMOURAnalyte/Calibration Date: Chloride/ 8-14-95

Concentration	Absorbance
x	y
0.000	0
20.000	86956
50.000	97307
100.000	212596
1000.000	2009766
5000.000	11642168

r	r <sup>2</sup>
0.9996	0.9992
slope	x intercept
2328.7286	23.6846
1/slope	y intercept
0.0004	-53243.732

**LINEAR REGRESSION ANALYSIS**

SDG: LK5106-LASDate: 17-Oct-95LATA No.: VB404.05Validator: BJ SEYMOURAnalyte/Calibration Date: Nitrate+Nitrite/ 8-18-95

Concentration	Absorbance
x	y
0.000	0
0.050	11
0.200	51
1.000	276
2.000	556
4.000	1095
8.010	2137

r	r <sup>2</sup>
0.9999	0.9998
slope	x intercept
267.6658	-0.0216
1/slope	y intercept
0.0037	5.9170

9613428.0910

LATA GENERAL CHEMISTRY  
CALCULATION SPREADSHEET

LINEAR REGRESSION ANALYSIS

SDG: LK5106-LAS

Date: 17-Oct-95

LATA No.: VB404.05

Validator: BJ SEYMOUR

Analyte/Calibration Date: Ammonia/ 8-16-95

Concentration	Absorbance
x	y
0.0000	0
0.0499	29
0.0992	50
0.4	175
1.6	722
6.4	3063

r  
0.9999

r<sup>2</sup>  
0.9998

slope  
478.5557

x intercept  
0.0185

1/slope  
0.0021

y intercept  
-8.703

9613428-0911

LATA GENERAL CHEMISTRY  
CALCULATION SPREADSHEET

PERCENT RECOVERY (ICV/CCV)

SDG: LK5106-LAS

Date: 17-Oct-95

LATA No.: VB404.05

Validator: BJ SEYMOUR

Analyte	Sample ID	Observed Value	True Value	%R
		O	A	
Chloride	ICV	994.558	1000	99%
Chloride	CCV	934.571	1000	93%
Ammonia	ICV	1.168	1.2	97.3%
Ammonia	CCV	1.615	1.600	100.9%
Nitrate+Nitrite	ICV	2.972	3.000	99.1%
Nitrate+Nitrite	CCV	3.994	4.000	99.9%
Sulfide	ICV	10.858	11.34	95.7%
Sulfide	CCV	18.755	19.90	94.2%

9613428.0912

LATA GENERAL CHEMISTRY  
CALCULATION SPREADSHEET

## MATRIX SPIKE RECOVERY (MS)

SDG: LK5106-LASDate: 17-Oct-95LATA No.: VB404.05Validator: BJ SEYMOUR

Analyte	Sample ID	Spike Sample Result	Sample Result	Spike Added	%R
		SSR	SR	SA	
Chloride	B0GFD7	68.98	27.107	40.00	105%
Ammonia	B0GFD7	4.847	0.455	4.00	109.8%
Nitrate+Nitrite	B0GFD7	39.301	35.162	4.00	103.5%
Sulfide	B0GFD7	7.206	0.000	7.960	90.5%

9613428-0913

LATA GENERAL CHEMISTRY  
CALCULATION SPREADSHEET

PERCENT RECOVERY (LCS)

SDG: LK5106-LAS

Date: 17-Oct-95

LATA No.: VB404.05

Validator: BJ SEYMOUR

Analyte	Observed value	True value	%R
	OLCS	ALCS	
Chloride	1019.943	1000.00	102%
Ammonia	4.246	4	106.2%
Nitrate+Nitrite	3.971	4	99.3%
Sulfide	5.725	7.96	71.9%

9613428.0914

LATA GENERAL CHEMISTRY  
CALCULATION SPREADSHEET

## RELATIVE PERCENT DIFFERENCE

SDG: LK5106-LASDate: 17-Oct-95LATA No.: VB404.05Validator: BJ SEYMOUR

Analyte	Sample ID	Original (Sample) concentration	Duplicate concentration	RPD
		OS	D	
<u>Chloride</u>	<u>B0GFD7</u>	<u>27.107</u>	<u>27.257</u>	1%
<u>Ammonia</u>	<u>B0GFD7</u>	<u>0.455</u>	<u>0.495</u>	8.4%
<u>Nitrate+Nitrite</u>	<u>B0GFD7</u>	<u>35.162</u>	<u>35.236</u>	0.2%
<u>Sulfide</u>	<u>B0GFD7</u>	<u>0.600</u>	<u>0.600</u>	0.0%

9613428.0915

LATA GENERAL CHEMISTRY  
CALCULATION SPREADSHEET

RESULTS CALCULATION, WATER

SDG: LK5106-LAS

Date: 17-Oct-95

LATA No.: VB404.05

Validator: BJ SEYMOUR

Analyte	Concentration from curve		Dilution Factor	Concentration (µg/L)
	CONCW	units	DFW	
<u>Chloride (B0GFD7)</u>	<u>27.107</u>	<u>mg/L</u>	<u>1</u>	27
<u>Ammonia (B0GFD7)</u>	<u>0.455</u>	<u>mg/L</u>	<u>1</u>	0.46
<u>Nitrate+Nitrite (B0GFD7)</u>	<u>35.162</u>	<u>mg/L</u>	<u>1</u>	35
<u>Sulfide (B0GFD7)</u>	<u>0.197</u>	<u>mg/L</u>	<u>1</u>	<1.0

9613428-0916

## Laboratory Case Narrative

Lockheed Analytical Services

Log-in No.: L5106  
 Quotation No.: Q400000-B  
 SAF: B95-068  
 Document File No.: 0811596  
 WHC Document File No.: 257  
 SDG No.: LK5106  
 Page 2

### CASE NARRATIVE INORGANIC NON METALS ANALYSES

The routine calibration and quality control analyses performed for this batch include as applicable: instrument tune (ICP/MS only), initial and continuing calibration verification, initial and continuing calibration blanks, method blank(s), laboratory control sample(s), ICP interference check samples (ICP only), serial dilutions, analytical (post-digestion) spike samples, matrix spike (predigestion) sample(s), duplicate sample(s).

#### Preparation and Analysis Requirements

- One water sample was received for LK5106 and analyzed in batch 811 bh for selected analytes as requested on the chain of custody. Quality control analysis was performed on the following sample:

Client ID	LAL #		Method
BOGFD7	L5106-3	MS, DUP	300.0 Chloride, Fluoride, Nitrate-Nitrogen, Nitrite-Nitrogen, Orthophosphate, Sulfate
	L5106-6	MS, DUP	350.1 Ammonia
	L5106-4	MS, DUP	353.2 Nitrate-Nitrite-Nitrogen
	L5106-5	MS, DUP	9030 Sulfide

#### Holding Time Requirements

- All samples were analyzed within the method-specific holding time with the exception of Method 300.0 Nitrate-Nitrogen, Nitrite-Nitrogen and Orthophosphate which were received outside of holding time. The associated samples are flagged with an "H".

#### Method Blanks

- The concentration levels of all the requested analytes in the method blank were below the reporting detection limits.

#### Internal Quality Control

- All Internal Quality Control were within acceptance limits.

Kay McCann  
 Prepared By

September 12, 1995  
 Date

000028

bis  
 10-17-95  
 0006

9613428.0918

## **Chain-of-Custody Information**

Bechtel Hanford, Inc.

# L5106

## CHAIN OF CUSTODY/SAMPLE ANALYSIS REQUEST

Data Turnaround

- Priority  
 Normal

Collector <i>K.D Lee</i>	Company Contact R. E. Peterson	Telephone (509) 372-9638
Project Designation 100-HR-3 Groundwater Sampling, Round 9, Phase 2	Sampling Location 100 D	SAF No. B95-068
Ice Chest No. <i>Patton</i>	Field Logbook No. <i>EFL-1018</i>	Method of Shipment Federal Express
Shipped To Lockheed	Offsite Property No. NA <sup>1045</sup> <i>W95-0-0204-46</i>	Bill of Lading/Air Bill No. <i>2904637303</i>

Possible Sample Hazards/Remarks	Preservation	HNO <sub>3</sub>	Cool 4°C	H <sub>2</sub> SO <sub>4</sub>	*1	H <sub>2</sub> SO <sub>4</sub>	HNO <sub>3</sub>	Cool 4°C	Cool 4°C		HNO <sub>3</sub>
	Type of Container	G	G	P/G	P	P/G	P/G	G	P/G		G
	No. of Container(s)	1	1	1	1	1	5	1	1		1
Special Handling and/or Storage Maintain samples between 2°C and 6°C.	Volume	500mL	500mL	500mL	1L	1L	1L	500mL	20mL		500mL
SAMPLE ANALYSIS	ICP Metals (Unfiltered)	Anions (IC) - F, Cl, SO <sub>4</sub> , NO <sub>2</sub> , NO <sub>3</sub> , PO <sub>4</sub>	NO <sub>2</sub> - NO <sub>3</sub>	Sulfide	Ammonia	Gross Alpha, Gross Beta, Sr-90	Tritium	Activity Scan		ICP Metals (Filtered)	

Sample No.	Matrix*	Date Sampled	Time Sampled								
BOGFD7	W	<i>8/9/95</i>	<i>1135</i>	<i>X</i>							
BOGFD8	W	<i>8/9/95</i>	<i>1135</i>								<i>X</i>

CHAIN OF POSSESSION		Sign/Print Names		SPECIAL INSTRUCTIONS *1 ZnAc + NaOH				Matrix*	
Relinquished By <i>K.D Lee</i>	Date/Time <i>8/10/95 0730</i>	Received By <i>BRE</i>	Date/Time <i>0730</i>	Sample analysis for phosphate, nitrate, and nitrite by EPA 300.0; and turbidity by EPA 180.1 is being requested for information only. The ERC Contractor acknowledges that the 48-hour holding time will not be met.  The Activity Scan is for all samples listed on this chain of custody.				<ul style="list-style-type: none"> <li>S - Soil</li> <li>SE - Sediment</li> <li>SO - Solid</li> <li>SL - Sludge</li> <li>W - Water</li> <li>O - Oil</li> <li>A - Air</li> <li>DS - Drum Solids</li> <li>DL - Drum Liquids</li> <li>T - Tissue</li> <li>WI - Wipe</li> <li>L - Liquid</li> <li>V - Vegetation</li> <li>X - Other</li> </ul>	
Relinquished By <i>BRE</i>	Date/Time <i>0830</i>	Received By <i>B. Whitten</i>	Date/Time <i>8-10-95</i>						
Relinquished By <i>B. Whitten</i>	Date/Time <i>8-10-95</i>	Received By	Date/Time						
Relinquished By <i>005</i>	Date/Time <i>0815</i>	Received By	Date/Time						
LABORATORY SECTION	Received By <i>ARM</i>	Title <i>Sample Custodian</i>		Date/Time <i>8-11-95 0900</i>					
FINAL SAMPLE DISPOSITION	Disposal Method		Disposed By				Date/Time		

7671200-0000

0000730

9613428.0920

## **Supplemental Information**

9613428-0921

LATA GENERAL CHEMISTRY  
DATA VALIDATION CHECKLIST

## INFORMATION REQUEST FORM (IRF)

To: Jeanette Duncan, WHC/BHIDate: 17-Oct-95Primary FAX: ~~372-2186~~ 9052

Secondary FAX: 372-1616

PROJECT NAME:	100-HR-3 ROUND 9
SDG NUMBER:	LK5106-LAS
LATA NO.:	VB404.05
LABORATORY:	LAS
CASE NUMBER:	N/A
ANALYSIS METHOD:	Chloride, Nitrate, Nitrite, Sulfate
ANALYSIS DATE:	8/14/95
ITEM(S) MISSING:	Raw Data for injection #15 (ICB) and injection# 22 (L5106-3)

Comments: This information is necessary to complete validation.Thankyou

RETURN TO LATA

Attention: BJ SEYMOURINFORMATION RECEIVED FROM WHC (INITIALS/DATE): bjs 10-31-95INFORMATION ACCEPTABLE?: YES  NO 

If NO is checked, send a new LIRF to request additional information.

Data Reprocessed On 10/30/1995 13:22:13

```

=====
Sample Name: L5106-3                               Date: 08/14/1995 12:42:48
Data File  : C:\ARCHIVE\AUGARC\081495\2811-BH1.D22
Method     : C:\DX\METHOD\ANIONSH2.MET
ACI Address: 1 System: 2 Inject#: 22                Detector: CDM-2
Analyst    :                                         Column:
=====
    
```


```

-----
Calibration Volume Dilution Points Rate Start Stop Area Reject
-----
External           1           1    2550  5Hz   0.00  8.50   100000
    
```

\*\*\*\*\* Component Report: All Components \*\*\*\*\*

PK. Num	Ret Time	Component Name	Concentration mg/L	Area	Height
1	1.62	CHLORIDE	27.107	372924634	68330012
0	0.00	NITRITE-NITROGEN	0.000	0	0
3	3.06	NITRATE-NITROGEN	35.228	1298196241	89955516
4	6.36	SULFATE	134.885	1379453750	64862742
Totals			197.220	3050574625	223148269

File: 2811-BH1.D22 Sample: L5106-3

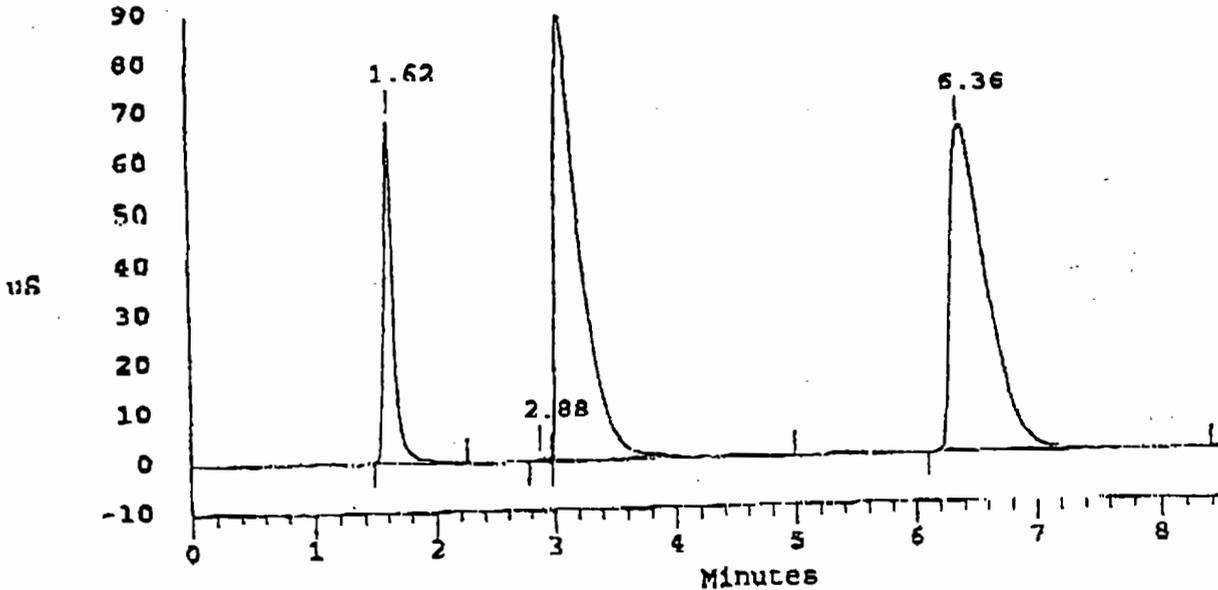

000033

9613428.0925

LOCKHEED ENGINEERING TEL:702-361-6434  
ANIONS BY ION CHROMATOGRAPHY  
METHOD 300.0/LAL-90-SOP-0019

Oct 30 95 16:53 No.016 P.04

Data Reprocessed On 10/30/1995 13:20:51

```

=====
Sample Name: ICB                               Date: 08/14/1995 10:25:14
Data File  : C:\ARCHIVE\CALCURV\95-226\20814951.D15
Method     : C:\DX\METHOD\ANIONSL2.MET
ACI Address: 1 System: 2 Inject#: 15           Detector: CDM-2
Analyst    :                               Column:
=====

```

```


-----
Calibration Volume Dilution Points Rate Start Stop Area Reject
-----
External           1             1 2550 SHz  0.00  8.50   20000
-----

```

\*\*\*\*\* Component Report: All Components \*\*\*\*\*

Pk. Num	Ret Time	Component Name	Concentration $\mu\text{g/L}$	Area	Height
0	0.00	CHLORIDE	0.000	0	0
1	1.91	NITRITE-NITROGEN	2.108	41532	3915
0	0.00	NITRATE-NITROGEN	0.000	0	0
0	0.00	SULFATE	0.000	0	0
Totals			2.108	41532	3915

File: 20814951.D15 Sample: ICB

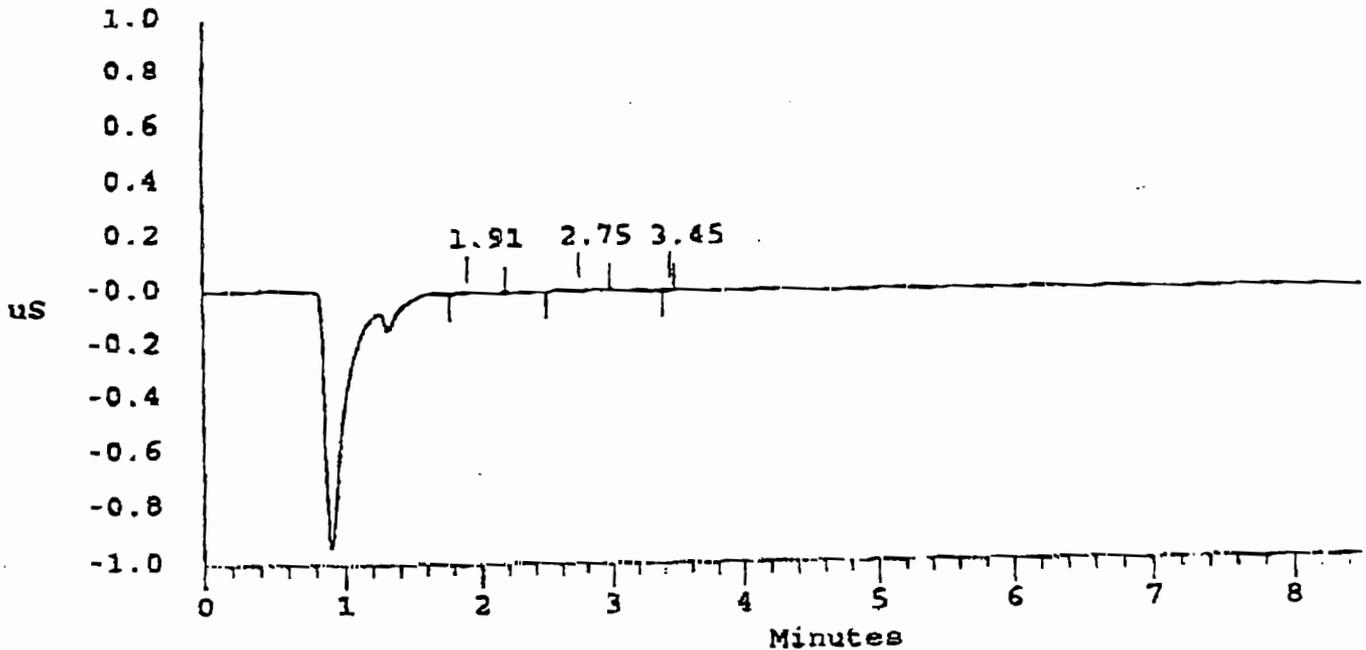

000034

9613428.0924

**END OF PACKAGE**

9613428.0925

**DATA VALIDATION REPORT**  
**for**  
**100-HR-3 GROUNDWATER ROUND 9**  
**PHASE II**  
**Radiochemistry Analysis**  
**SDG LK5106-LAS**  
**LATA VB404.05**

Bechtel Hanford Inc.  
P.O. Box 969  
Richland, Washington

November 10, 1995

## Table of Contents

Data Validation Narrative .....	000002
INTRODUCTION .....	000002
ANALYSES REQUESTED .....	000002
DATA QUALITY OBJECTIVES .....	000002
REFERENCES .....	000004
GLOSSARY OF VALIDATION APPLIED QUALIFIERS (RADIOCHEMISTRY) ..	000005
GLOSSARY OF LABORATORY APPLIED QUALIFIERS .....	000006
Qualification Summary Table .....	000007
Data Summary Table .....	000009
Sample Results .....	000011
Checklist .....	000014
Laboratory Case Narrative .....	000025
Chain-of-Custody Information .....	000027
Supplemental Information .....	000030
END OF PACKAGE .....	000032

**100-HR-3 GROUNDWATER ROUND 9 PHASE II  
Data Validation Narrative**

**INTRODUCTION**

All samples in Sample Delivery Group (SDG) LK5106-LAS (VB404.05) were validated at level D as defined in the Data Validation Procedures for Radiochemical Analyses (WHC-SD-EN-SPP-001, Rev. 1)

The analyses were performed by Lockheed Analytical Services.

**ANALYSES REQUESTED**

See Table 1.

**DATA QUALITY OBJECTIVES**

**Precision:** Goals for precision were met.

**Accuracy:** Goals for accuracy were met.

**Sample Result Verification:** All sample results were supported in the raw data.

**Detection Limits:** Detection limit goals were met for all sample results as specified in the *RCRA Facility Investigative/Corrective Measures Study Work Plan for the 100-HR-3 Operable Unit*, DOE/RL-88-36, Rev. 0.

**Completeness:** The data package was 100% complete for all requested analyses.

**MAJOR DEFICIENCIES**

No major deficiencies were identified during data validation which required qualification of data as unusable.

**MINOR DEFICIENCIES**

No minor deficiencies were identified during data validation which required qualification of data as estimated.

**Table 1**  
**Chain-of-Custody**  
**Analysis Request**

LATA ID #: VB404.05

SDG: LK5106-LAS

Sample Information				Analyses Requested					
SAMPLE NO.	DATE COLLECTED	MATRIX	FIELD QC INFO	1	2	3	4	5	6
				B0GFD7	9-Aug-95	WATER	Split of B0GFB1	X	X

**Method References:**

	<u>Analysis</u>	<u>Method</u>
1.	Gross Alpha	LAL-91-SOP-0060
2.	Gross Beta	LAL-91-SOP-0060
3.	Total Strontium	LAL-91-SOP-0196
4.	Tritium	LAL-91-SOP-0066
5.	Activity Scan	Lab Specific
6.	Rad Screen	Lab Specific

**NOTES:** (complete documentation of these notes can be found in the Supplemental Information Section of this report)

## NOTE 1:

The rad screen was deemed unnecessary prior to off-site shipment.

**REFERENCES**

WHC 1993, *Data Validation Procedures for Radiochemical Analyses*, WHC-SD-EN-SPP-001, Rev. 1, Westinghouse Hanford Company, Richland, Washington.

DOE 1992, *RCRA Facility Investigation/Corrective Measures Study Plan for the 100-HR-3 Operable Unit*, DOE/RL-88-36, Rev. 0, Department of Energy-Hanford, Richland, Washington.

**GLOSSARY OF VALIDATION APPLIED QUALIFIERS (RADIOCHEMISTRY)**

Qualifiers which may be applied by data validators in compliance with the procedures herein are as follows.

- U- Indicates the constituent was analyzed for, but was not detected at a concentration above the Minimum Detectable Activity (MDA). The concentration reported is the sample result corrected for sample aliquot size, dilution factors, and percent solids (in the case of solid matrices) by the laboratory. The associated data should be considered usable for decision making purposes.
- UJ- Indicates the constituent was analyzed for and was not detected at a concentration above the Minimum Detectable Activity (MDA). Due to a quality control deficiency identified during data validation, the result reported may not accurately reflect the sample concentration. The associated data should be considered usable for decision making purposes.
- J- Indicates a constituent was analyzed for and detected. The associated value is estimated due to a quality control deficiency identified during validation. The data should be considered usable for decision making purposes.
- R- Indicates the constituent was analyzed for and detected; however, due to an identified quality control deficiency the data should be considered unusable for decision making purposes.
- UR- Indicates the constituent was analyzed for and not detected; however, due to an identified quality control deficiency the data should be considered unusable for decision making purposes.

**GLOSSARY OF LABORATORY APPLIED QUALIFIERS**

Qualifiers which may be applied by the laboratory in compliance with applicable requirements are as follows.

Commonly used laboratory radiochemistry qualifiers:

- U- Indicates the analyte was analyzed for but not detected in the sample.
- J- Indicates the value reported is estimated due to the presence of interference.
- C- Indicates the presence of high Total Dissolved Solids in the sample required reduction of sample size which increased the MDA.

9613428.0932

## Qualification Summary Table

9613428.0933

Qualification Summary Table

Radiochemistry

ANALYTE	TYPE	QUALIFIER	SAMPLES AFFECTED	DQO	REASON
No qualifiers were assigned by the validator.					

**Comments:**

1. The field split RPD values will be evaluated in SDG # W0663-QES, LATA ID VB404.07.
2. The MDA for the Gross Alpha analysis is greater than the RDL .

000008

9613428.0934

## Data Summary Table

9613428.0935

RADIOCHEMISTRY  
DATA SUMMARY TABLE

LATA ID#: VB404.05		HEIS #:	B0GFD7	
		Date:	9-Aug-95	
		Matrix:	WATER	
Constituent	CAS #	Units	Results	Q
Gross Alpha	ALPHA	pCi/L	3.7	
Gross Beta	BETA	pCi/L	11.3	
Strontium-90	10098-97-2	pCi/L	4.37	
Tritium	10028-17-8	pCi/L	3680	

000010

Shaded areas indicate changes by the validator.  
40405DST.XLS, RADIOCHEMISTRY

10/18/95, 11:07

9613428.0936

## Sample Results (Form I's)

9613428.0937

LOCKHEED ANALYTICAL SERVICES

RAD DATA REPORT (ra01)

Bechtel Hanford, Inc. \* Richland, WA

Bechtel Hanford Project (Project BECHTEL-HANFORD)

Client Sample ID: B0GFD7

LAL Sample ID: L5106-7

Date Collected: 09-AUG-95

Date Received: 11-AUG-95

Matrix: Water

Login Number: L5106

Constituent	Analyzed	Batch	Activity	Error	MDA	DataQual	Units
Gross Alpha	23-AUG-95	GR ALP/BETA LAL-0060_26272	3.7	2.6	3.5	C	pCi/L
Gross Beta	23-AUG-95	GR ALP/BETA LAL-0060_26272	11.3	2.7	3.4		pCi/L
Total radio-strontium	18-AUG-95	SR-90 LAL-0196_26273	4.37	0.63	0.72		pCi/L

*AA*  
*10-18-95*

9613428.0938

LOCKHEED ANALYTICAL SERVICES

RAD DATA REPORT (ra01)

Bechtel Hanford, Inc. \* Richland, WA

Bechtel Hanford Project (Project BECHTEL-HANFORD)

Client Sample ID: B0GFD7

LAL Sample ID: L5106-12

Date Collected: 09-AUG-95

Date Received: 11-AUG-95

Matrix: Water

Login Number: L5106

Constituent	Analyzed	Batch	Activity	Error	MDA	DataQual	Units
H-3	24-AUG-95	TRITIUM(H3) LAL-0066_26274	3680	480	270		pCi/L

*AF*  
*10-18-95*

9613428.0939

# Checklist

9613428.0940

LATA RADIOCHEMISTRY  
DATA VALIDATION CHECKLIST

VALIDATION LEVEL:	A	B	C	D	E
VALIDATION PROCEDURE:	<input type="checkbox"/> WHC-CM-5-3, Rev. 0		<input checked="" type="checkbox"/> WHC-SD-EN-SPP-001, Rev. 1		

PROJECT:	100-HR-3	SDG:	LK5106-LAS
VALIDATOR:	AM FREIER	LATA NO:	VB404.05
REVIEWER:	BJ MORRIS	LAB:	LAS
SAF NO:	B95-068	QAPP NO:	DOE/RL-88-36, Rev. 0
		SAP NO:	N/A

ANALYSES REQUESTED			
<input checked="" type="checkbox"/>	Gross Alpha/Beta LAL-91-SOP-0060	<input checked="" type="checkbox"/>	Total Strontium LAL-91-SOP-0196
<input checked="" type="checkbox"/>		<input checked="" type="checkbox"/>	Tritium LAL-91-SOP-0066
SAMPLE NO.	MATRIX	COMMENTS:	
BOGFD7	WATER		

**1. DATA PACKAGE COMPLETENESS AND CASE NARRATIVE** YES NO N/A

Is technical verification documentation present?

Is a case narrative present?

**2. HOLDING TIMES** YES NO N/A

Are sample holding times acceptable?

Are samples preserved correctly?

See HOLDING TIME SUMMARY form

**3. INSTRUMENT PERFORMANCE AND CALIBRATIONS** YES NO N/A

Were instruments/detectors calibrated within one year of sample analysis?

Are initial calibrations acceptable?

Are standards NIST traceable?

Are standards acceptable?

**Comments:** Calibration of instruments/detectors was not performed within one year of sample analysis, however continuing calibration data is acceptable. Therefore, no qualifiers are assigned.

9613428.0941

LATA RADIOCHEMISTRY  
DATA VALIDATION CHECKLIST

4. CONTINUING CALIBRATION

YES NO N/A

Background checked at proper frequency?

Background check acceptable?

Efficiency checked at proper frequency?

Efficiency check acceptable?

Calibration check standards NIST traceable?

Calibration check standards acceptable?

If NO(s) are checked, see CALIBRATION DATA SUMMARY form

5. BLANKS

YES NO N/A

Were method blanks analyzed?

Are the method blanks free of analytes?

Were method blank results acceptable?

Validation calculation/transcription checks were performed and are acceptable.

If NO(s) are checked, see BLANK DATA SUMMARY form

6. ACCURACY

YES NO N/A

Were spike samples analyzed at the proper frequency?

Are all spike sample recoveries acceptable?

Were laboratory control standards (LCS) analyzed at the proper frequency?

Are all LCS recoveries acceptable?

Was a tracer/chemical carrier added?

Was the tracer/chemical carrier recovery acceptable?

Are standard sources traceable?

Are standards acceptable?

Validation calculation checks were performed and are acceptable.

If NO(s) are checked, see ACCURACY DATA SUMMARY form

9613428.0942

LATA RADIOCHEMISTRY  
DATA VALIDATION CHECKLIST

7. PRECISION	YES	NO	N/A
Were laboratory duplicates analyzed at the proper frequency?	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Are all duplicate RPD values acceptable?	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Validation calculation checks were performed and are acceptable.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>

**If NO(s) are checked, see PRECISION DATA SUMMARY form**

8. FIELD QC SAMPLES	YES	NO	N/A
Were field QC samples (field/trip blanks, duplicates, splits, performance audit) identified?	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Are field/trip blank results acceptable? (see Blank Data Summary form)	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
Are field duplicate RPD values acceptable? (see Field QC calculations)	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
Are field split RPD values acceptable? (see Field QC calculations)	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
Are performance audit sample results acceptable?	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>

**Comments:** Sample BOGFD7 is a field split of B0GFB1.  
 The field split RPD values will be evaluated in SDG # W0663-QES, LATA ID VB404.07.

9. REPORTED RESULTS AND DETECTION LIMITS	YES	NO	N/A
Are results reported for all requested analyses?	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Are all results supported in the raw data?	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Are results calculated properly?	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Do MDAs meet the RDLs?	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>
Validation calculation checks were performed and are acceptable.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>

**Comments:** The MDA for the Gross Alpha analysis is greater than the RDL.

**VALIDATION SUMMARY**

For deficiencies (major and minor) and comments, please refer to the Qualification Summary Table.

9613428.0943

LATA RADIOCHEMISTRY  
DATA VALIDATION CHECKLIST

## HOLDING TIME SUMMARY

SDG: LK5106-LAS		VALIDATOR: AM FREIER					DATE: 18-Oct-95			
PROJECT: 100-HR-3		REVIEWER: BJ MORRIS					LATA NO.: VB404.05			
HEIS-SN	MATRIX CODE	ANALYSIS	DATE COLLECTED	PREP DATE	ANALYSIS DATE	PREP HT (days)	<i>Required HT (days)</i>	ANALYSIS HT (days)	<i>Required HT (days)</i>	VAL Q
B0GFD7	WATER	Gross Alpha/Beta	9-Aug-95	N/A	23-Aug-95	N/A	<i>N/A</i>	14	<i>180</i>	NONE
B0GFD7	WATER	Strontium	9-Aug-95	N/A	18-Aug-95	N/A	<i>N/A</i>	9	<i>180</i>	NONE
B0GFD7	WATER	Tritium	9-Aug-95	N/A	24-Aug-95	N/A	<i>N/A</i>	15	<i>180</i>	NONE

9613428.0944

LATA RADIOCHEMISTRY  
CALCULATION SPREADSHEET

MATRIX SPIKE RECOVERY (MS)

SDG: LK5106-LAS

Date: 18-Oct-95

LATA No.: VB404.05

Validator: AM FREIER

Analyte	Sample ID	Spike Sample Result	Sample Result	Spike Added	%R
Gross Alpha	B0GFD7	46.2	3.71	48.8	87%
Gross Beta	B0GFD7	65	11.3	50.3	107%
Tritium	B0GFD7	6730	3680	3580	85%

9613428.0945

LATA RADIOCHEMISTRY  
CALCULATION SPREADSHEET

PERCENT RECOVERY (LCS)

SDG: LK5106-LAS

Date: 18-Oct-95

LATA No.: VB404.05

Validator: AM FREIER

Analyte	Observed value	True value	%R
Gross Alpha	44.6	39.2	114%
Gross Beta	42.4	42.5	100%
Strontium	47.7	51.8	92%
Tritium	2360	2260	104%

9613428.0946

LATA RADIOCHEMISTRY  
CALCULATION SPREADSHEET

## RELATIVE PERCENT DIFFERENCE

SDG: LK5106-LASDate: 18-Oct-95LATA No.: VB404.05Validator: AM FREIER

Analyte	Sample ID	Original (Sample) concentration	Duplicate concentration	RPD
Gross Alpha	B0GFD7	3.71	1.86	66.4%
Gross Beta	B0GFD7	11.30	14.20	22.7%
Strontium	B0GFD7	4.37	3.14	32.8%
Tritium	B0GFD7	3680	3520	4.44%

9613429.0947

LATA RADIOCHEMISTRY  
CALCULATION SPREADSHEET

## MINIMUM DETECTABLE ACTIVITY (MDA)

SDG: LK5106-LASDate: 18-Oct-95LATA No.: VB404.05Validator: AM FREIER

Analyte	Sample ID	Bkgmd counts/ min (cpm) or Std Dev of bkgmd (cpm)	Count time for assoc. sample	Detector Efficiency	Ingrowth corr. factor	Tracer/ Carrier recovery factor	Decay factor	Chemical yield factor	Sample volume (L or g)	MDA
Gross Alpha	BOGFD7	0.04	100	0.09	1.00	1.00	1.00	1.00	0.165	3.46
Gross Beta	BOGFD7	1.01	100	0.40	1.00	1.00	1.00	1.00	0.17	3.40
Strontium	BOGFD7	0.98	200	0.45	1.00	0.90	1.00	1.00	0.50	0.72
Tritium	BOGFD7	0.90	20	0.18	1.00	1.00	1.00	1.00	0.01	279

9613428.0948

LATA RADIOCHEMISTRY  
CALCULATION SPREADSHEET

## RESULTS CALCULATION GROSS ALPHA/BETA AND TRITIUM

SDG: LK5106-LASDate: 18-Oct-95LATA No.: VB404.05Validator: AM FREIER

Analyte	Gross Counts per minute	Background Counts per minute	Activity of alpha fraction in beta channel	Detector Efficiency	Sample volume (L or g)	Result
Gross Alpha	0.16	0.04	1.00	0.09	0.17	3.72
Gross Beta	2.69	1.01	1.00	0.40	0.17	11.53
Tritium	16.03	0.90	1.00	0.18	0.01	3765.37

9613428.0949

LATA RADIOCHEMISTRY  
CALCULATION SPREADSHEET

RESULTS CALCULATION TOTAL STRONTIUM

SDG: LK5106-LAS

Date: 18-Oct-95

LATA No.: VB404.05

Validator: AM FREIER

Analyte	Gross Counts per minute	Background Counts per minute	Ingrowth correction Factor	Detector Efficiency	Carrier recovery factor	Strontium decay factor	Sample volume (L or g)	Result
Strontium-90	3.03	0.98	1.00	0.45	0.90	1.00	0.50	4.54

9613428.0950

## Laboratory Case Narrative

**Lockheed Analytical Services**

Log-in No.: L5106  
Quotation No.: Q400000-B  
SAF: B95-068  
Document File No.: 0811596  
WHC Document File No.: 257  
SDG No.: LK5106  
Page 5

## CASE NARRATIVE RADIOCHEMICAL ANALYSES

The routine calibration and quality control (QC) analyses performed for this batch include as applicable: instrument calibration, initial and continuing calibration verification, quench monitoring standards, instrument background analysis, method blanks, yield tracer, laboratory control samples, matrix spike samples, duplicate samples.

**NOTE:** Chemical recoveries and minimum detectable activities can be found on the preparation sheets and calculation sheets on the attached raw data for each method.

### Holding Time Requirements

All holding times were met.

### Analytical Method Gross Alpha/Beta

The gross alpha/beta analysis was performed using standard operating procedure (SOP), LAL-91-SOP-0060. The samples were analyzed in workgroup 26272. No problems were encountered during analysis and all QC criteria were met. No re-analyses were performed.

### Analytical Method Strontium-90

The strontium-90 analysis was performed using SOP, LAL-91-SOP-0196. The samples were analyzed in workgroup 26273. No problems were encountered during the analysis and all QC criteria were met with the following exceptions: The relative error recovery and relative percent difference were slightly out of QC criteria. Data quality is not adversely affected. No re-analyses were performed.

### Analytical Method Tritium

The tritium analysis was performed using SOP, LAL-91-SOP-0066. The samples were analyzed in workgroup 26274. No problems were encountered during analysis and all QC criteria were met. No re-analyses were performed.

Andrea Tippett  
Prepared By

August 26, 1995  
Date

000026

AS  
10-18-95  
0009

9613428.0952

## **Chain-of-Custody Information**

Bechtel Hanford, Inc.

# L5106

## CHAIN OF CUSTODY/SAMPLE ANALYSIS REQUEST

Data Turnaround

- Priority
- Normal

Collector <i>K-D Lee</i>	Company Contact R. E. Peterson	Telephone (509) 372-9638
Project Designation 100-HR-3 Groundwater Sampling, Round 9, Phase 2	Sampling Location 100 D	SAF No. B95-068
Ice Chest No. <i>Patton</i>	Field Logbook No. <i>E.F.L-1018</i>	Method of Shipment Federal Express
Shipped To Lockheed	Offsite Property No. NA <sup>SW</sup> <del>8-10-95</del> <i>W95-0-0204-46</i>	Bill of Lading/Air Bill No. <i>2904637303</i>

Possible Sample Hazards/Remarks	Preservation	HNO <sub>3</sub>	Cool 4°C	H <sub>2</sub> SO <sub>4</sub>	*1	H <sub>2</sub> SO <sub>4</sub>	HNO <sub>3</sub>	Cool 4°C	Cool 4°C		HNO <sub>3</sub>
	Type of Container	G	G	P/G	P	P/G	P/G	G	P/G		G
	No. of Container(s)	1	1	1	1	1	5	1	1		1
Special Handling and/or Storage Maintain samples between 2°C and 6°C.	Volume	500mL	500mL	500mL	1L	1L	1L	500mL	20mL		500mL
SAMPLE ANALYSIS	ICP Metals (Unfiltered)	Anions (IC) - F, Cl, SO <sub>4</sub> , NO <sub>2</sub> , NO <sub>3</sub> , PO <sub>4</sub>	NO <sub>2</sub> - NO <sub>3</sub>	Sulfide	Ammonia	Gross Alpha, Gross Beta, Sr-90	Tritium	Activity Scan			ICP Metals (Filtered)

Sample No.	Matrix*	Date Sampled	Time Sampled									
BOGFD7	W	<i>8/9/95</i>	<i>1135</i>	<i>X</i>								
BOGFD8	W	<i>8/9/95</i>	<i>1135</i>									<i>X</i>

CHAIN OF POSSESSION		Sign/Print Names		SPECIAL INSTRUCTIONS				Matrix*	
Relinquished By <i>Kolee</i> Date/Time <i>8/10/95 0730</i>		Received By <i>BRC</i> Date/Time <i>0730</i>		*1 ZnAc + NaOH  Sample analysis for phosphate, nitrate, and nitrite by EPA 300.0; and turbidity by EPA 180.1 is being requested for information only. The ERC Contractor acknowledges that the 48-hour holding time will not be met.  The Activity Scan is for all samples listed on this chain of custody.				<ul style="list-style-type: none"> <li>S - Soil</li> <li>SE - Sediment</li> <li>SO - Solid</li> <li>SL - Sludge</li> <li>W - Water</li> <li>O - Oil</li> <li>A - Air</li> <li>DS - Drum Solids</li> <li>DL - Drum Liquids</li> <li>T - Tissue</li> <li>WI - Wipe</li> <li>L - Liquid</li> <li>V - Vegetation</li> <li>X - Other</li> </ul>	
Relinquished By <i>K.D. Lee</i> Date/Time <i>8-10-95 0830</i>		Received By <i>B. Whitten</i> Date/Time <i>8-10-95</i>							
Relinquished By <i>K.D. Lee</i> Date/Time <i>8-10-95</i>		Received By <i>B. Whitten</i> Date/Time <i>8-10-95</i>							
Relinquished By <i>K.D. Lee</i> Date/Time <i>8-11-95</i>		Received By <i>B. Whitten</i> Date/Time <i>8-11-95</i>							
LABORATORY SECTION	Received By <i>K.D. Lee</i>	Title <i>Sample Custodian</i>		Date/Time <i>8-11-95 0900</i>					
FINAL SAMPLE DISPOSITION	Disposal Method <i>000028</i>	Disposed By <i>K.D. Lee</i>		Date/Time <i>8-11-95 0900</i>					

7191154

Lockheed Analytical Services  
Sample Receiving Checklist

Client Name: *Bechtel - Hanford*

Job No. *LS104*

Cooler ID:

COOLER CONDITION UPON RECEIPT

Temperature of cooler upon receipt: *2°C*

temperature of temp. blank upon receipt:

	Yes	No	* Comments/Discrepancies
custody seals intact	<input checked="" type="checkbox"/>		
chain of custody present	<input checked="" type="checkbox"/>		
blue ice (or equiv.) present/frozen	<input checked="" type="checkbox"/>		
rad survey completed	<input checked="" type="checkbox"/>		

SAMPLE CONDITION UPON RECEIPT

	Yes	No	* Comments/Discrepancies
all bottles labeled	<input checked="" type="checkbox"/>		
samples intact	<input checked="" type="checkbox"/>		
proper container used for sample type	<input checked="" type="checkbox"/>		
sample volume sufficient for analysis	<input checked="" type="checkbox"/>		
proper pres. indicated on the COC	<input checked="" type="checkbox"/>		
VOA's contain headspace			<i>nh</i>
are samples bi-phasic (if so, indicate sample ID'S):			<i>NA</i>

MISCELLANEOUS ITEMS

	Yes	No	* Comments/Discrepancies
samples with short holding times		<input checked="" type="checkbox"/>	
samples to subcontract		<input checked="" type="checkbox"/>	

ADDITIONAL COMMENTS/DISCREPANCIES

Completed by / date: *[Signature]* *8-11-95*

Sent to the client (date/initials):

\*\* Client's signature upon receipt:

Notes: \* = contact the appropriate CSR of any discrepancies immediately upon receipt

\*\* = please review this information and return via facsimile to the appropriate CSR (702) 361-8146

000029

*[Handwritten notes and signatures]*

9613428-0954

9613428.0955

## Supplemental Information

Environmental Restoration Contractor **ERC Team**  
**Interoffice Memorandum**

Job No. 22192  
Written Response Required: NO  
CCN: N/A  
OU: 100-HR-3  
TSD: N/A  
ERA: N/A  
Subject Code: 9830

TO: W. S. Thompson N3-06 DATE: July 26, 1995

COPIES: R. L. Biggerstaff H4-91 FROM: S. K. De Mers  
Radiological Controls  
T7-05/373-1913

SUBJECT: 1995 Phase 2, Round 9 sampling for 100-HR-3

There is no need to perform total activities prior to offsite shipment to NRC licensed labs of samples taken from the attached list of wells.

All wells listed in the attachment were reviewed for radiological content based on the previous 4 years of sampling data. No well listed has a  $\beta$  activity in excess of 100,000 pCi/l (< .1 uCi/sample based on a 1 liter sample size) nor any  $\alpha$  activity in excess of 10,000 pCi/l (< .01 uCi/l based on a 1 liter sample). All wells show activities < 2,000 pCi/gm (< 2 nCi/gm D.O.T. limit). The highest activity in recent samples is 73 pCi/l  $\beta$  and 10 pCi/l  $\alpha$ .

Radiological monitoring during sampling will only be required if the wells are located in radiological areas or if the wells themselves are labeled with radiological stickers. Monitoring requirements for down hole work such as pump removal will be determined based on the history of each well on a case by case basis.

Copies: T. L. Lafreniere X0-23  
K. F. Trapp N3-05 N1-28

DELAYED DUE TO  
INCORRECT MSIN  
PLEASE NOTIFY SENDER

Attachment - 1995 Phase 2, Round 9 well list for 100 HR-3  
skd

AJ  
10-18-95

0016

000031

511596

9613428.0957

**END OF PACKAGE**